



US008083671B2

(12) **United States Patent**  
**Boulais et al.**

(10) **Patent No.:** **US 8,083,671 B2**  
(45) **Date of Patent:** **Dec. 27, 2011**

(54) **FLUID DELIVERY SYSTEM FOR USE WITH AN ENDOSCOPE**

(75) Inventors: **Dennis R Boulais**, Danielson, CT (US);  
**Michael S Banik**, Bolton, MA (US);  
**Vincent Turturro**, Bolton, MA (US);  
**Christopher Rowland**, Hopkinton, MA (US);  
**David W Hoffman**, Concord, MA (US);  
**John P O'Connor**, Andover, MA (US);  
**Eric Litscher**, Hopkinton, MA (US)

(73) Assignee: **Boston Scientific Scimed, Inc.**, Maple Grove, MN (US)

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1282 days.

(21) Appl. No.: **11/239,644**

(22) Filed: **Sep. 29, 2005**

(65) **Prior Publication Data**

US 2006/0106285 A1 May 18, 2006

**Related U.S. Application Data**

(60) Provisional application No. 60/614,868, filed on Sep. 30, 2004.

(51) **Int. Cl.**  
**A61B 1/12** (2006.01)

(52) **U.S. Cl.** ..... **600/158**; 600/156; 600/131

(58) **Field of Classification Search** ..... 600/156-159, 600/104, 130-132, 139

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

3,266,059 A 8/1966 Stelle  
3,470,876 A 10/1969 Barchilon

3,572,325 A 3/1971 Bazell et al.  
3,581,738 A 6/1971 Moore  
4,108,211 A 8/1978 Tanaka  
4,286,585 A 9/1981 Ogawa  
4,294,162 A 10/1981 Fowler et al.  
4,311,134 A \* 1/1982 Mitsui et al. .... 600/158  
4,315,309 A 2/1982 Coli  
4,351,323 A 9/1982 Ouchi et al.  
4,402,310 A \* 9/1983 Kimura ..... 600/158  
4,425,113 A 1/1984 Bilstad  
4,432,349 A 2/1984 Oshiro  
4,471,766 A 9/1984 Terayama  
4,473,841 A 9/1984 Murakoshi et al.  
4,488,039 A 12/1984 Sato et al.  
4,491,865 A 1/1985 Danna et al.

(Continued)

**FOREIGN PATENT DOCUMENTS**

EP 0 075 153 B1 3/1983

(Continued)

*Primary Examiner* — John P Leubecker


*Assistant Examiner* — Victoria Chen

(74) *Attorney, Agent, or Firm* — Finnegan, Henderson, Farabow, Garrett & Dunner, LLP

(57) **ABSTRACT**

A fluid delivery system for use with an endoscope. Certain embodiments of the invention include a single, large fluid source and pump installed upon an operator console, in combination with a small fluid reservoir and pump installed within a proximal connector of the imaging endoscope, multiple fluid sources that feed a common fluid channel that are pressurized by a common pump, multiple fluid sources that feed dedicated fluid channels that are pressurized by dedicated pumps, and a small fluid reservoir and pump installed within a handheld manual controller of the imaging endoscope. The fluid delivery endoscopic systems of the present invention provide the user with the flexibility of changing fluids either in advance of a procedure or on-the-fly as needed, instead of relying on fixed fluid sources only.

**18 Claims, 19 Drawing Sheets**

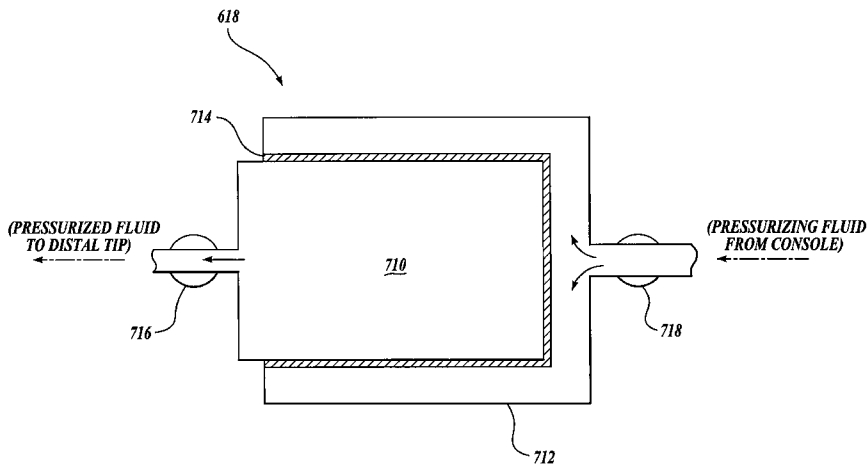

U.S. PATENT DOCUMENTS		
4,493,537 A	1/1985	Nakahashi
4,495,134 A	1/1985	Ouchi et al.
4,499,895 A	2/1985	Takayama
4,503,842 A	3/1985	Takayama
4,513,235 A	4/1985	Acklam et al.
4,515,444 A	5/1985	Prescott et al.
4,516,063 A	5/1985	Kaye et al.
4,519,391 A	5/1985	Murakoshi
4,552,130 A *	11/1985	Kinoshita ..... 600/158
4,559,928 A	12/1985	Takayama
4,566,437 A	1/1986	Yamaguchi
4,573,450 A	3/1986	Arakawa
4,580,210 A	4/1986	Nordstrom
4,586,923 A	5/1986	Gould et al.
4,615,330 A	10/1986	Nagasaki et al.
4,616,630 A	10/1986	Arakawa
4,617,915 A	10/1986	Arakawa
4,618,884 A	10/1986	Nagasaki
4,621,618 A	11/1986	Omagari et al.
4,622,584 A	11/1986	Nagasaki et al.
4,625,714 A	12/1986	Toyota
4,631,582 A	12/1986	Nagasaki et al.
4,633,303 A	12/1986	Nagasaki et al.
4,633,304 A	12/1986	Nagasaki
4,643,170 A	2/1987	Miyazaki et al.
4,646,723 A	3/1987	Arakawa
4,649,904 A	3/1987	Krauter et al.
4,651,202 A	3/1987	Arakawa
4,652,093 A	3/1987	Stephen et al.
4,652,916 A	3/1987	Suzaki et al.
4,654,701 A	3/1987	Yabe
RE32,421 E	5/1987	Hattori
4,662,725 A	5/1987	Nisioka
4,663,657 A	5/1987	Nagasaki et al.
4,667,655 A *	5/1987	Ogiu et al. .... 600/132
4,674,844 A	6/1987	Nishioka et al.
4,686,963 A	8/1987	Cohen et al.
4,697,210 A	9/1987	Toyota et al.
4,700,693 A	10/1987	Lia et al.
4,714,075 A	12/1987	Krauter et al.
4,716,457 A	12/1987	Matsuo
4,719,508 A	1/1988	Sasaki et al.
4,727,417 A	2/1988	Kanno et al.
4,727,418 A	2/1988	Kato et al.
4,745,470 A	5/1988	Yabe et al.
4,745,471 A	5/1988	Takamura et al.
4,746,974 A	5/1988	Matsuo
4,748,970 A	6/1988	Nakajima
4,755,029 A	7/1988	Okobe
4,762,119 A	8/1988	Allred et al.
4,765,312 A	8/1988	Sasa et al.
4,766,489 A	8/1988	Kato
4,787,369 A	11/1988	Allred et al.
4,790,294 A	12/1988	Allred et al.
4,794,913 A	1/1989	Shimonaka et al.
4,796,607 A	1/1989	Allred et al.
4,800,869 A	1/1989	Nakajima
4,805,596 A	2/1989	Hatori
4,806,011 A	2/1989	Bettinger
4,819,065 A	4/1989	Eino
4,819,077 A	4/1989	Kikuchi et al.
4,821,116 A	4/1989	Nagasaki et al.
4,824,225 A	4/1989	Nishioka
4,831,437 A	5/1989	Nishioka et al.
4,836,187 A	6/1989	Iwakoshi et al.
4,844,052 A	7/1989	Iwakoshi et al.
4,844,071 A	7/1989	Chen et al.
4,845,553 A	7/1989	Konomura et al.
4,845,555 A	7/1989	Yabe et al.
4,847,694 A	7/1989	Nishihara
4,853,772 A	8/1989	Kikuchi
4,860,731 A	8/1989	Matsuura
4,867,546 A	9/1989	Nishioka et al.
4,868,647 A	9/1989	Uehara et al.
4,869,237 A	9/1989	Eino et al.
4,873,965 A	10/1989	Danieli
4,875,468 A	10/1989	Krauter et al.
4,877,314 A	10/1989	Kanamori
4,882,623 A	11/1989	Uchikubo
4,884,134 A	11/1989	Tsuji et al.
4,885,634 A	12/1989	Yabe
4,890,159 A	12/1989	Ogiu
4,894,715 A	1/1990	Uchikubo et al.
4,895,431 A	1/1990	Tsujiuchi et al.
4,897,789 A	1/1990	King et al.
4,899,731 A	2/1990	Takayama et al.
4,899,732 A	2/1990	Cohen
4,899,787 A	2/1990	Ouchi et al.
4,905,666 A	3/1990	Fukuda
4,918,521 A	4/1990	Yabe et al.
4,919,112 A	4/1990	Siegmund
4,919,114 A	4/1990	Miyazaki
4,920,980 A	5/1990	Jackowski
4,928,172 A	5/1990	Uehara et al.
4,931,867 A	6/1990	Kikuchi
4,941,454 A	7/1990	Wood et al.
4,941,456 A	7/1990	Wood et al.
4,951,134 A	8/1990	Nakasima et al.
4,951,135 A	8/1990	Sasagawa et al.
4,952,040 A	8/1990	Igarashi
4,960,127 A	10/1990	Noce et al.
4,961,110 A	10/1990	Nakamura
4,967,269 A	10/1990	Sasagawa et al.
4,971,034 A	11/1990	Doi et al.
4,973,311 A	11/1990	Iwakoshi et al.
4,979,497 A	12/1990	Matsuura et al.
4,982,725 A	1/1991	Hibino et al.
4,984,878 A	1/1991	Miyano
4,986,642 A	1/1991	Yokota et al.
4,987,884 A	1/1991	Nishioka et al.
4,989,075 A	1/1991	Ito
4,989,581 A	2/1991	Tamburrino et al.
4,996,974 A	3/1991	Ciarlei
4,996,975 A	3/1991	Nakamura
5,001,556 A	3/1991	Nakamura et al.
5,005,558 A	4/1991	Aomori
5,005,957 A	4/1991	Kanamori et al.
5,007,408 A	4/1991	Ieoka
5,018,509 A	5/1991	Suzuki et al.
5,022,382 A	6/1991	Ohshoki et al.
5,029,016 A	7/1991	Hiyama et al.
5,034,888 A	7/1991	Uehara et al.
5,040,069 A	8/1991	Matsumoto et al.
RE33,689 E	9/1991	Nishioka et al.
5,045,935 A	9/1991	Kikuchi
5,049,989 A	9/1991	Tsuji
5,050,584 A	9/1991	Matsuura
5,050,974 A	9/1991	Takasugi et al.
5,056,503 A	10/1991	Nagasaki
5,061,994 A	10/1991	Takahashi
5,068,719 A	11/1991	Tsuji
5,074,861 A	12/1991	Schneider et al.
5,081,524 A	1/1992	Tsuruoka et al.
5,087,989 A	2/1992	Igarashi
5,110,645 A	5/1992	Matsumoto et al.
5,111,281 A	5/1992	Sekiguchi
5,111,306 A	5/1992	Kanno et al.
5,111,804 A	5/1992	Funakoshi
5,113,254 A	5/1992	Kanno et al.
5,115,136 A *	5/1992	Tomasch ..... 250/461.1
5,119,238 A	6/1992	Igarashi
5,131,393 A	7/1992	Ishiguro et al.
5,137,013 A	8/1992	Chiba et al.
5,140,265 A	8/1992	Sakiyama et al.
5,159,446 A	10/1992	Hibino et al.
5,170,775 A	12/1992	Tagami
5,172,225 A	12/1992	Takahashi et al.
5,174,293 A	12/1992	Hagiwara
5,176,629 A	1/1993	Kullas et al.
5,191,878 A	3/1993	Iida et al.
5,198,931 A	3/1993	Igarashi
5,201,908 A	4/1993	Jones
5,208,702 A	5/1993	Shiraiwa
5,209,220 A	5/1993	Hiyama et al.
5,225,958 A	7/1993	Nakamura
5,228,356 A	7/1993	Chuang
5,243,416 A	9/1993	Nakazawa

5,243,967	A	9/1993	Hibino		5,767,839	A	6/1998	Rosenberg	
5,257,628	A	11/1993	Ishiguro et al.		5,779,686	A	7/1998	Sato et al.	
5,267,956	A	12/1993	Beuchat	604/30	5,781,172	A	7/1998	Engel et al.	
5,271,381	A	12/1993	Ailinger et al.		5,785,521	A	7/1998	Rizoiu et al.	433/29
RE34,504	E	1/1994	Uehara et al.		5,788,714	A	8/1998	Ouchi	
5,291,010	A	3/1994	Tsuji		5,789,047	A	8/1998	Sasaki et al.	
5,297,537	A	3/1994	Savitt et al.	600/158	5,793,539	A	8/1998	Konno et al.	
5,299,559	A	4/1994	Bruce et al.		5,805,140	A	9/1998	Rosenberg et al.	
5,311,858	A	5/1994	Adair		5,810,715	A	9/1998	Moriyama	
5,325,845	A	7/1994	Adair et al.		5,812,983	A	9/1998	Kumagai	
5,331,551	A	7/1994	Tsuruoka et al.		5,819,736	A	10/1998	Avny et al.	
5,342,299	A	8/1994	Snoke et al.		5,820,591	A	10/1998	Thompson et al.	
5,343,855	A	9/1994	Iida et al.	600/157	5,821,466	A	10/1998	Clark et al.	
5,347,989	A	9/1994	Monroe et al.		5,821,920	A	10/1998	Rosenberg et al.	
5,374,953	A	12/1994	Sasaki et al.		5,823,948	A	10/1998	Ross, Jr. et al.	
5,379,757	A	1/1995	Hiyama et al.		5,827,186	A	10/1998	Chen et al.	
5,381,782	A	1/1995	DeLaRama et al.		5,827,190	A	10/1998	Palcic et al.	
5,390,662	A	2/1995	Okada		5,828,197	A	10/1998	Martin et al.	
5,400,769	A	3/1995	Tanii et al.		5,828,363	A	10/1998	Yaniger et al.	
5,402,768	A	4/1995	Adair		5,830,124	A	11/1998	Suzuki et al.	
5,402,769	A	4/1995	Tsuji		5,830,128	A	11/1998	Tanaka	
5,409,485	A	4/1995	Suda		5,830,180	A	11/1998	Chandler et al.	604/65
5,412,478	A	5/1995	Ishihara et al.		5,833,935	A	11/1998	Malchesky	422/300
5,418,649	A	5/1995	Igarashi		5,836,869	A	11/1998	Kudo et al.	
5,419,772	A	5/1995	Teitz et al.	604/141	5,837,023	A	11/1998	Koike et al.	
5,420,644	A	5/1995	Watanabe		5,840,014	A	11/1998	Miyano et al.	
5,431,645	A	7/1995	Smith et al.		5,841,126	A	11/1998	Fossom et al.	
5,434,615	A	7/1995	Matsumoto		5,843,000	A	12/1998	Nishioka et al.	
5,436,640	A	7/1995	Reeves		5,846,183	A	12/1998	Chilcoat	
5,436,767	A	7/1995	Suzuki et al.		5,855,560	A	1/1999	Idaomi et al.	
5,440,341	A	8/1995	Suzuki et al.		5,857,963	A	1/1999	Pelchy et al.	
5,464,007	A	11/1995	Krauter et al.		5,865,724	A	2/1999	Palmer et al.	
5,469,840	A	11/1995	Tanii et al.		5,868,664	A	2/1999	Speier et al.	
5,473,235	A	12/1995	Lance et al.		5,868,666	A	2/1999	Okada et al.	
5,482,029	A	1/1996	Sekiguchi et al.		5,873,816	A	2/1999	Kagawa et al.	
5,484,407	A	1/1996	Osyypka		5,873,866	A	2/1999	Kondo et al.	
5,485,316	A	1/1996	Mori et al.		5,876,326	A	3/1999	Takamura et al.	
5,496,260	A	3/1996	Krauter et al.		5,876,331	A	3/1999	Wu et al.	
5,515,449	A	5/1996	Tsuruoka et al.		5,876,373	A	3/1999	Giba et al.	
5,518,501	A	5/1996	Oneda et al.		5,876,427	A	3/1999	Chen et al.	
5,518,502	A	5/1996	Kaplan et al.		5,877,819	A	3/1999	Branson	
5,543,831	A	8/1996	Tsuji et al.		5,879,284	A	3/1999	Tsujita	
5,569,158	A	10/1996	Suzuki et al.		5,880,714	A	3/1999	Rosenberg et al.	
5,569,159	A	10/1996	Anderson et al.		5,882,293	A	3/1999	Ouchi	
5,586,262	A	12/1996	Komatsu et al.		5,882,339	A	3/1999	Beiser et al.	
5,589,854	A	12/1996	Tsai		5,889,670	A	3/1999	Schuler et al.	
5,591,202	A	1/1997	Slater et al.		5,889,672	A	3/1999	Schuler et al.	
5,605,545	A	2/1997	Nowosielski et al.	604/118	5,892,630	A	4/1999	Broome	
5,608,451	A	3/1997	Konno et al.		5,895,350	A	4/1999	Hori	
5,619,380	A	4/1997	Agasawa et al.		5,897,507	A	4/1999	Kortenbach et al.	
5,622,528	A	4/1997	Hamano et al.		5,897,525	A	4/1999	Dey et al.	
5,631,695	A	5/1997	Nakamura et al.		5,907,487	A	5/1999	Rosenberg et al.	
5,633,203	A	5/1997	Adair		5,923,018	A	7/1999	Kameda et al.	
5,643,203	A	7/1997	Beiser et al.		5,928,136	A	7/1999	Barry	
5,645,075	A	7/1997	Palmer et al.		5,929,607	A	7/1999	Rosenberg et al.	
5,647,840	A	7/1997	D'Amelio et al.		5,929,846	A	7/1999	Rosenberg et al.	
5,658,238	A	8/1997	Suzuki et al.		5,929,900	A	7/1999	Yamanaka	
5,667,477	A	9/1997	Segawa		5,929,901	A	7/1999	Adair et al.	
5,674,182	A	10/1997	Suzuki et al.		5,931,833	A	8/1999	Silverstein	
5,674,197	A	10/1997	van Muiden et al.		5,933,809	A	8/1999	Hunt et al.	
5,685,823	A	11/1997	Ito et al.		5,935,085	A	8/1999	Welsh et al.	
5,685,825	A	11/1997	Takase et al.		5,936,778	A	8/1999	Miyano et al.	
5,691,853	A	11/1997	Miyano		5,941,817	A	8/1999	Crawford	
5,695,450	A	12/1997	Yabe et al.		5,950,168	A	9/1999	Simborg et al.	
5,698,866	A	12/1997	Doiron et al.		5,951,462	A	9/1999	Yamanaka	
5,701,155	A	12/1997	Wood		5,951,779	A	9/1999	Koyanagi et al.	134/2
5,702,349	A	12/1997	Morizumi		5,956,416	A	9/1999	Tsuruoka et al.	
5,702,754	A	12/1997	Zhong		5,956,689	A	9/1999	Everhart	
5,703,724	A	12/1997	Miyano		5,956,690	A	9/1999	Haggerson et al.	
5,704,371	A	1/1998	Shepard		5,959,613	A	9/1999	Rosenberg et al.	
5,704,896	A	1/1998	Fukunishi et al.		5,976,070	A	11/1999	Ono et al.	
5,708,482	A	1/1998	Takahashi et al.		5,976,074	A	11/1999	Moriyama	
5,721,566	A	2/1998	Rosenberg et al.		5,980,454	A	11/1999	Broome	
5,724,068	A	3/1998	Sanchez et al.		5,980,468	A	11/1999	Zimmon	
5,728,045	A	3/1998	Komi		5,986,693	A	11/1999	Adair et al.	
5,739,811	A	4/1998	Rosenberg et al.		5,991,729	A	11/1999	Barry et al.	
5,740,801	A	4/1998	Branson		5,991,730	A	11/1999	Lubin et al.	
5,746,696	A	5/1998	Kondo		5,999,168	A	12/1999	Rosenberg et al.	
5,764,809	A	6/1998	Nomami et al.		6,002,425	A	12/1999	Yamanaka et al.	

6,007,482 A	12/1999	Madni et al.	6,441,845 B1	8/2002	Matsumoto
6,007,531 A	12/1999	Snoke et al.	6,447,444 B1	9/2002	Avni et al.
6,014,630 A	1/2000	Jeacock et al.	6,449,006 B1	9/2002	Shipp
6,015,088 A	1/2000	Parker et al.	6,453,190 B1	9/2002	Acker et al.
6,017,322 A	1/2000	Snoke et al.	6,454,162 B1	9/2002	Teller
6,020,875 A	2/2000	Moore et al.	6,459,447 B1	10/2002	Okada et al.
6,020,876 A	2/2000	Rosenberg et al.	6,468,204 B2	10/2002	Sendai et al.
6,026,363 A	2/2000	Shepard	6,475,141 B2	11/2002	Abe
6,030,360 A	2/2000	Biggs	6,478,730 B1	11/2002	Bala et al.
6,032,120 A	2/2000	Rock et al.	6,489,987 B1	12/2002	Higuchi et al.
6,039,728 A	3/2000	Berlien et al.	6,496,827 B2	12/2002	Kozam et al.
6,043,839 A	3/2000	Adair et al.	6,498,948 B1	12/2002	Ozawa et al.
6,050,718 A	4/2000	Schena et al.	6,503,193 B1	1/2003	Iwasaki et al.
6,057,828 A	5/2000	Schena et al.	6,520,908 B1	2/2003	Ikeda et al.
6,059,719 A	5/2000	Yamamoto et al.	6,524,234 B2	2/2003	Ouchi
6,061,004 A	5/2000	Rosenberg	6,530,882 B1	3/2003	Farkas et al.
6,067,077 A	5/2000	Martin et al.	6,533,722 B2	3/2003	Nakashima
6,071,248 A	6/2000	Zimmon	6,540,669 B2	4/2003	Abe et al.
6,075,555 A	6/2000	Street	6,544,194 B1	4/2003	Kortenbach et al.
6,078,308 A	6/2000	Rosenberg et al.	6,545,703 B1	4/2003	Takahashi et al.
6,078,353 A	6/2000	Yamanaka et al.	6,551,239 B2	4/2003	Renner et al.
6,078,876 A	6/2000	Rosenberg et al.	6,558,317 B2	5/2003	Takahashi et al.
6,080,104 A	6/2000	Ozawa et al.	6,561,971 B1	5/2003	Akiba
6,081,809 A	6/2000	Kumagai	6,565,507 B2	5/2003	Kamata et al.
6,083,152 A	7/2000	Strong	6,569,087 B2*	5/2003	Naito et al. .... 600/156
6,083,170 A	7/2000	Ben-Haim	6,574,629 B1	6/2003	Cooke, Jr. et al.
6,095,971 A	8/2000	Takahashi	6,589,162 B2	7/2003	Nakashima et al.
6,099,465 A	8/2000	Inoue	6,595,913 B2	7/2003	Takahashi
6,100,874 A	8/2000	Schena et al.	6,597,390 B1	7/2003	Higuchi
6,104,382 A	8/2000	Martin et al.	6,599,239 B2	7/2003	Hayakawa et al.
6,120,435 A	9/2000	Eino	6,602,186 B1	8/2003	Sugimoto et al.
6,125,337 A	9/2000	Rosenberg et al.	6,605,035 B2	8/2003	Ando et al.
6,128,006 A	10/2000	Rosenberg et al.	6,609,135 B1	8/2003	Omori et al.
6,132,369 A	10/2000	Takahashi	6,611,846 B1	8/2003	Stoodley
6,134,056 A	10/2000	Nakamura	6,614,969 B2	9/2003	Eichelberger et al.
6,134,506 A	10/2000	Rosenberg et al.	6,616,601 B2	9/2003	Hayakawa
6,135,946 A	10/2000	Konen et al.	6,623,424 B2	9/2003	Hayakawa et al.
6,139,508 A	10/2000	Simpson et al.	6,638,214 B2	10/2003	Akiba
6,141,037 A	10/2000	Upton et al.	6,638,215 B2	10/2003	Kobayashi
6,142,956 A	11/2000	Kortenbach et al.	6,641,528 B2	11/2003	Torii
6,146,355 A	11/2000	Biggs	6,651,669 B1	11/2003	Burnside
6,149,607 A	11/2000	Simpson et al.	6,656,110 B1	12/2003	Irion et al.
6,152,877 A	11/2000	Masters	6,656,112 B2	12/2003	Miyanaga
6,154,198 A	11/2000	Rosenberg	6,659,940 B2	12/2003	Adler
6,154,248 A	11/2000	Ozawa et al.	6,663,561 B2	12/2003	Sugimoto et al.
6,155,988 A	12/2000	Peters	6,669,629 B2	12/2003	Matsui
6,181,481 B1	1/2001	Yamamoto et al.	6,673,012 B2	1/2004	Fujii et al.
6,184,922 B1	2/2001	Saito et al.	6,677,984 B2	1/2004	Kobayashi et al.
6,193,714 B1	2/2001	McGaffigan et al.	6,678,397 B1	1/2004	Omori et al.
6,195,592 B1	2/2001	Schuler et al.	6,682,479 B1	1/2004	Takahashi et al.
6,203,493 B1	3/2001	Ben-Haim	6,685,631 B2	2/2004	Minami
6,206,824 B1	3/2001	Ohara et al.	6,686,949 B2	2/2004	Kobayashi et al.
6,211,904 B1	4/2001	Adair	6,690,409 B1	2/2004	Takahashi
6,216,104 B1	4/2001	Moshfeghi et al.	6,690,963 B2	2/2004	Ben-Haim et al.
6,219,091 B1	4/2001	Yamanaka et al.	6,692,431 B2	2/2004	Kazakevich
6,221,070 B1	4/2001	Tu et al.	6,697,101 B1	2/2004	Takahashi et al.
6,234,958 B1*	5/2001	Snoke et al. .... 600/114	6,699,181 B2	3/2004	Wako
6,238,799 B1	5/2001	Opolski	6,702,737 B2	3/2004	Hinto et al.
6,241,668 B1	6/2001	Herzog	6,711,426 B2	3/2004	Benaron et al.
6,260,994 B1	7/2001	Matsumoto et al.	6,715,068 B1	3/2004	Kazunori
6,272,470 B1	8/2001	Teshima	6,716,162 B2	4/2004	Hakamata
6,275,255 B1	8/2001	Adair et al.	6,728,599 B2	4/2004	Wang et al.
6,283,960 B1	9/2001	Ashley	6,730,018 B2	5/2004	Takase
6,295,082 B1	9/2001	Dowdy et al.	6,736,773 B2	5/2004	Wendlandt et al.
6,299,625 B1	10/2001	Bacher	6,743,240 B2	6/2004	Smith et al.
6,309,347 B1	10/2001	Takahashi et al.	6,749,559 B1	6/2004	Kraas et al.
6,310,642 B1	10/2001	Adair et al.	6,749,560 B1	6/2004	Konstorum et al.
6,319,196 B1	11/2001	Minami	6,749,561 B2	6/2004	Kazakevich
6,319,197 B1	11/2001	Tsuji et al.	6,753,905 B1	6/2004	Okada et al.
6,334,844 B1	1/2002	Akiba	6,758,806 B2	7/2004	Kamrava et al.
6,346,075 B1	2/2002	Arai et al.	6,758,807 B2	7/2004	Minami
6,366,799 B1	4/2002	Acker et al.	6,758,842 B2	7/2004	Irion et al.
6,381,029 B1	4/2002	Tipirneni	6,778,208 B2	8/2004	Takeshige et al.
6,398,724 B1	6/2002	May et al.	6,780,151 B2	8/2004	Grabover et al.
6,413,207 B1	7/2002	Minami	6,785,410 B2	8/2004	Vining et al.
6,421,078 B1	7/2002	Akai et al.	6,785,414 B1	8/2004	McStravick et al.
6,425,535 B1	7/2002	Akiba	6,785,593 B2	8/2004	Wang et al.
6,425,858 B1	7/2002	Minami	6,796,938 B2	9/2004	Sendai
6,436,032 B1	8/2002	Eto et al.	6,796,939 B1	9/2004	Hirata et al.

6,798,533 B2	9/2004	Tipirneni	6,980,227 B2	12/2005	Iida et al.
6,800,056 B2	10/2004	Tartaglia et al.	6,980,921 B2	12/2005	Anderson et al.
6,800,057 B2	10/2004	Tsujita et al.	6,981,945 B1	1/2006	Sarvazyan et al.
6,808,491 B2	10/2004	Kortenbach et al.	6,982,740 B2	1/2006	Adair et al.
6,824,539 B2	11/2004	Novak	6,984,206 B2	1/2006	Kumei et al.
6,824,548 B2	11/2004	Smith et al.	6,985,183 B2	1/2006	Jan et al.
6,829,003 B2	12/2004	Takami	6,986,686 B2	1/2006	Shibata et al.
6,830,545 B2	12/2004	Bendall	6,994,668 B2	2/2006	Miyano
6,832,990 B2	12/2004	Kortenbach et al.	6,994,704 B2	2/2006	Qin et al.
6,840,932 B2	1/2005	Lang et al.	6,997,883 B1 *	2/2006	Hahn ..... 600/560
6,842,196 B1	1/2005	Swift et al.	7,001,330 B2	2/2006	Kobayashi
6,846,286 B2	1/2005	Suzuki et al.	7,008,376 B2	3/2006	Ikeda et al.
6,847,933 B1	1/2005	Hastings	7,204,821 B1 *	4/2007	Clare et al. .... 604/30
6,849,043 B2	2/2005	Kondo	7,413,542 B2 *	8/2008	Kucklick et al. .... 600/156
6,850,794 B2	2/2005	Shahidi	2001/0039370 A1	11/2001	Takahashi et al.
6,855,109 B2	2/2005	Obata et al.	2001/0049491 A1	12/2001	Shimada
6,858,004 B1	2/2005	Ozawa et al.	2002/0017515 A1	2/2002	Obata et al.
6,858,014 B2	2/2005	Damarati	2002/0028984 A1	3/2002	Hayakawa et al.
6,860,849 B2	3/2005	Matsushita et al.	2002/0055669 A1	5/2002	Konno
6,863,650 B1	3/2005	Irion	2002/0080248 A1	6/2002	Adair et al.
6,863,661 B2	3/2005	Carrillo et al.	2002/0087048 A1	7/2002	Brock et al.
6,868,195 B2	3/2005	Fujita	2002/0087166 A1	7/2002	Brock et al.
6,871,086 B2	3/2005	Nevo et al.	2002/0095175 A1	7/2002	Brock et al.
6,873,352 B2	3/2005	Mochida et al.	2002/0128633 A1	9/2002	Brock et al.
6,876,380 B2	4/2005	Abe et al.	2002/0177802 A1 *	11/2002	Moutafis et al. .... 604/22
6,879,339 B2	4/2005	Ozawa	2002/0193662 A1	12/2002	Belson
6,881,188 B2	4/2005	Furuya et al.	2002/0193664 A1	12/2002	Ross et al.
6,882,785 B2	4/2005	Eichelberger et al.	2003/0032862 A1 *	2/2003	Ota et al. .... 600/158
6,884,392 B2 *	4/2005	Malkin et al. .... 422/26	2003/0034863 A1	2/2003	Kazakevich
6,887,195 B1	5/2005	Pilvisto	2003/0065250 A1	4/2003	Chiel et al.
6,890,294 B2	5/2005	Niwa et al.	2003/0069897 A1	4/2003	Roy et al.
6,892,090 B2	5/2005	Verard et al.	2003/0133011 A1	7/2003	Amling
6,892,112 B2	5/2005	Wang et al.	2003/0135252 A1 *	7/2003	MacHold et al. .... 607/106
6,895,268 B1	5/2005	Rahn et al.	2003/0149338 A1	8/2003	Francois et al.
6,898,086 B2	5/2005	Takami et al.	2003/0181905 A1	9/2003	Long
6,899,673 B2	5/2005	Ogura et al.	2004/0049097 A1	3/2004	Miyake
6,899,674 B2	5/2005	Viebach et al.	2004/0054258 A1	3/2004	Maeda et al.
6,899,705 B2	5/2005	Niemeyer	2004/0073083 A1	4/2004	Ikeda et al.
6,900,829 B1	5/2005	Ozawa et al.	2004/0073084 A1	4/2004	Maeda et al.
6,902,527 B1	6/2005	Doguchi et al.	2004/0073085 A1	4/2004	Ikeda et al.
6,902,529 B2	6/2005	Onishi et al.	2004/0143159 A1	7/2004	Wendlandt
6,903,761 B1	6/2005	Abe et al.	2004/0147809 A1	7/2004	Kazakevich
6,903,883 B2	6/2005	Amanai	2004/0167379 A1	8/2004	Akiba
6,905,057 B2	6/2005	Swayze et al.	2004/0193017 A1 *	9/2004	Akiba ..... 600/156
6,905,462 B1	6/2005	Homma	2004/0249247 A1	12/2004	Iddan
6,908,427 B2	6/2005	Fleener et al.	2004/0257608 A1	12/2004	Tipirneni
6,908,429 B2	6/2005	Heimberger et al.	2005/0192476 A1	9/2005	Homan et al.
6,911,916 B1	6/2005	Wang et al.	2005/0197861 A1	9/2005	Omori et al.
6,916,286 B2	7/2005	Kazakevich	2005/0200698 A1	9/2005	Amling et al.
6,923,818 B2	8/2005	Muramatsu et al.	2005/0203341 A1	9/2005	Welker et al.
6,928,490 B1	8/2005	Buchholz et al.	2005/0203418 A1	9/2005	Yamada et al.
6,929,602 B2 *	8/2005	Hirakui et al. .... 600/159	2005/0205958 A1	9/2005	Taniguchi et al.
6,930,706 B2	8/2005	Kobayashi et al.	2005/0207645 A1	9/2005	Nishimura et al.
6,932,761 B2	8/2005	Maeda et al.	2005/0209509 A1	9/2005	Belson
6,934,093 B2	8/2005	Kislev et al.	2005/0225872 A1	10/2005	Uzawa et al.
6,934,575 B2	8/2005	Ferre et al.	2005/0226508 A1	10/2005	Gotohda
6,943,663 B2	9/2005	Wang et al.	2005/0228221 A1	10/2005	Hirakawa
6,943,821 B2	9/2005	Abe et al.	2005/0228222 A1	10/2005	Furumi
6,943,822 B2	9/2005	Iida et al.	2005/0228227 A1	10/2005	Weber
6,943,946 B2	9/2005	Fiete	2005/0228697 A1	10/2005	Funahashi
6,943,959 B2	9/2005	Homma	2005/0231591 A1	10/2005	Abe
6,943,966 B2	9/2005	Konno	2005/0234507 A1	10/2005	Geske et al.
6,944,031 B2	9/2005	Takami et al.	2005/0243169 A1	11/2005	Ono et al.
6,949,068 B2	9/2005	Taniguchi et al.	2005/0247081 A1	11/2005	Sakata et al.
6,950,248 B2	9/2005	Rudischhauser et al.	2005/0250983 A1	11/2005	Tremaglio et al.
6,950,691 B2	9/2005	Uchikubo	2005/0251112 A1	11/2005	Danitz et al.
6,954,311 B2	10/2005	Amanai	2005/0251998 A1	11/2005	Bar-Or et al.
6,955,671 B2	10/2005	Uchikubo	2005/0253044 A1	11/2005	Kuriyama
6,956,703 B2	10/2005	Saito	2005/0256370 A1	11/2005	Fujita
6,961,187 B2	11/2005	Amanai	2005/0256373 A1	11/2005	Bar-Or et al.
6,962,564 B2	11/2005	Hickle	2005/0256377 A1	11/2005	Deppmeier et al.
6,963,175 B2	11/2005	Archenhold et al.	2005/0256424 A1	11/2005	Zimmon
6,964,662 B2	11/2005	Kidooka et al.	2005/0264687 A1	12/2005	Murayama
6,967,673 B2	11/2005	Ozawa et al.	2005/0267417 A1	12/2005	Secrest et al.
6,974,466 B2	12/2005	Ahmed et al.	2005/0271340 A1	12/2005	Weisburg et al.
6,975,968 B2	12/2005	Nakamitsu et al.	2005/0272978 A1	12/2005	Brunnen et al.
6,976,954 B2	12/2005	Takahashi	2005/0273085 A1	12/2005	Hinmane et al.
6,977,053 B2	12/2005	Mukasa et al.	2005/0288545 A1	12/2005	Matsumoto et al.
6,977,670 B2	12/2005	Takahashi et al.	2005/0288553 A1	12/2005	Sugimoto


2006/0015008 A1 1/2006 Kennedy  
 2006/0047185 A1\* 3/2006 Shener et al. .... 600/156  
 2006/0047186 A1\* 3/2006 Annecke ..... 600/159  
 2006/0068360 A1 3/2006 Boulais  
 2006/0074346 A1\* 4/2006 Hibner ..... 600/566  
 2006/0122586 A1\* 6/2006 Geiselhart ..... 606/10  
 2007/0043262 A1\* 2/2007 Levy et al. .... 600/156

JP 07-8441 A 1/1995  
 JP 3482238 B2 12/1995  
 JP 10-113330 A 5/1998  
 JP 10-286221 A 10/1998  
 JP 11-216113 A 8/1999  
 JP 2001 128933 A 5/2001  
 JP 2002 078675 A 3/2002  
 JP 2002-102152 A 4/2002  
 JP 2002-177197 A 6/2002  
 JP 2002-185873 A 6/2002  
 JP 2002-253481 A 9/2002  
 JP 2003-75113 A 3/2003  
 JP 2002 007134 A 7/2003  
 WO WO 93/13704 A1 7/1993  
 WO WO 2004/016310 A2 2/2004  
 WO WO 2005/023082 A2 3/2005  
 WO 2006039512 A1 4/2006

FOREIGN PATENT DOCUMENTS

EP 0 437 229 A1 7/1991  
 EP 0 689 851 A1 1/1996  
 EP 0 728 487 B1 8/1996  
 EP 1 300 883 A2 4/2003  
 JP 05-31071 A 2/1993  
 JP 05-091972 A 4/1993  
 JP 06-105800 4/1994  
 JP 3372273 B2 4/1994  
 JP 06-254048 A 9/1994  
 JP 3219521 B2 9/1994

\* cited by examiner

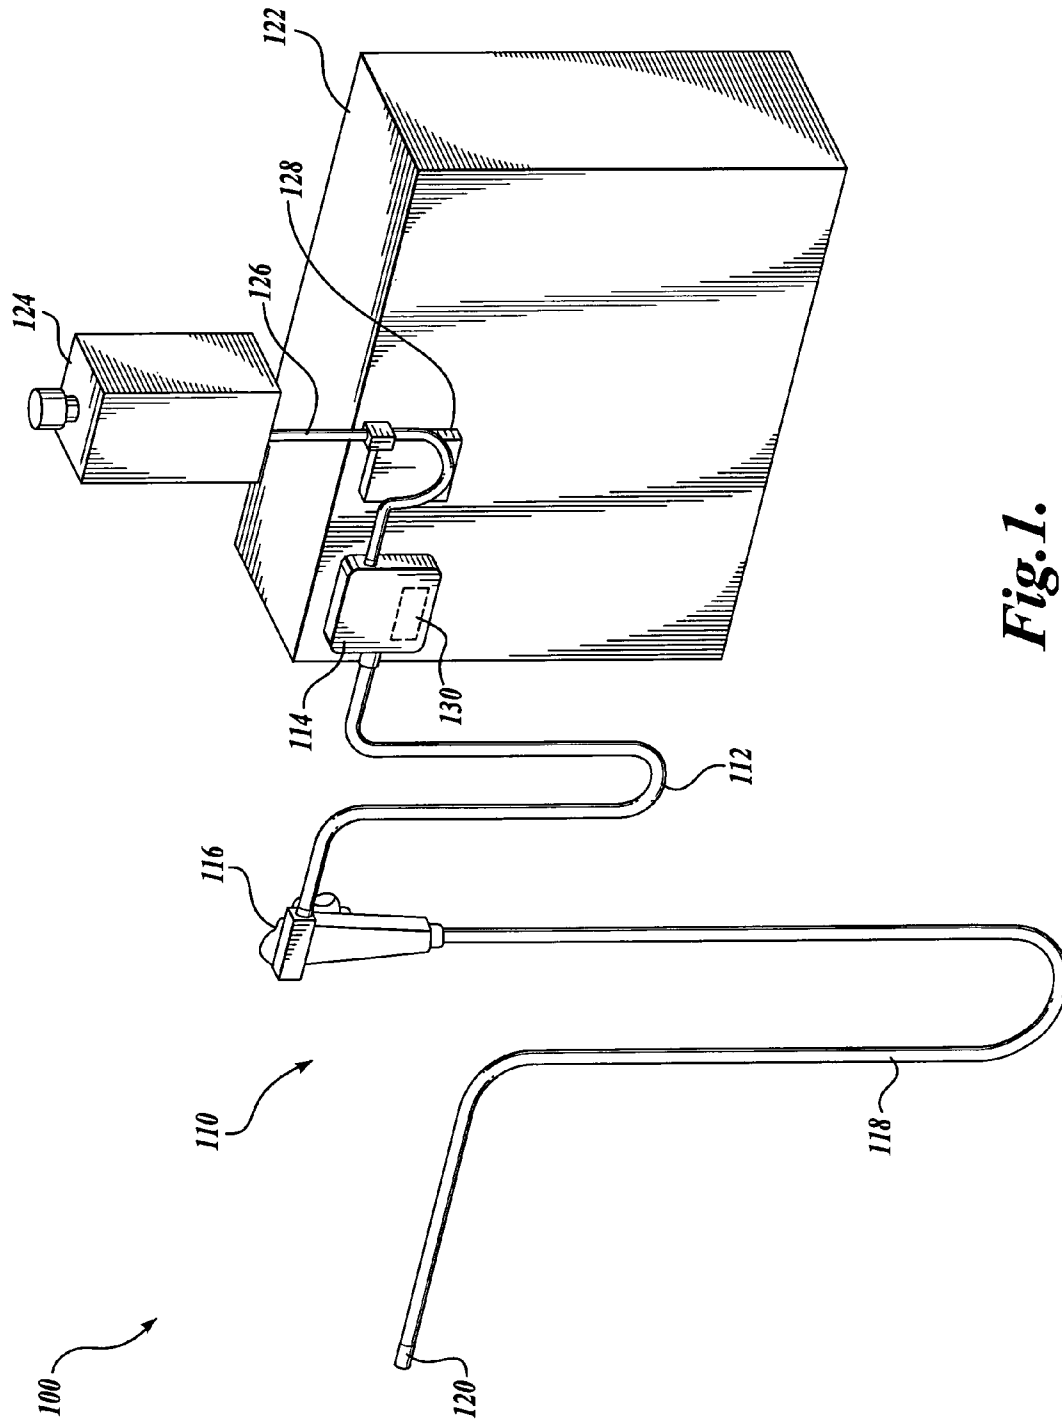

**Fig. 1.**


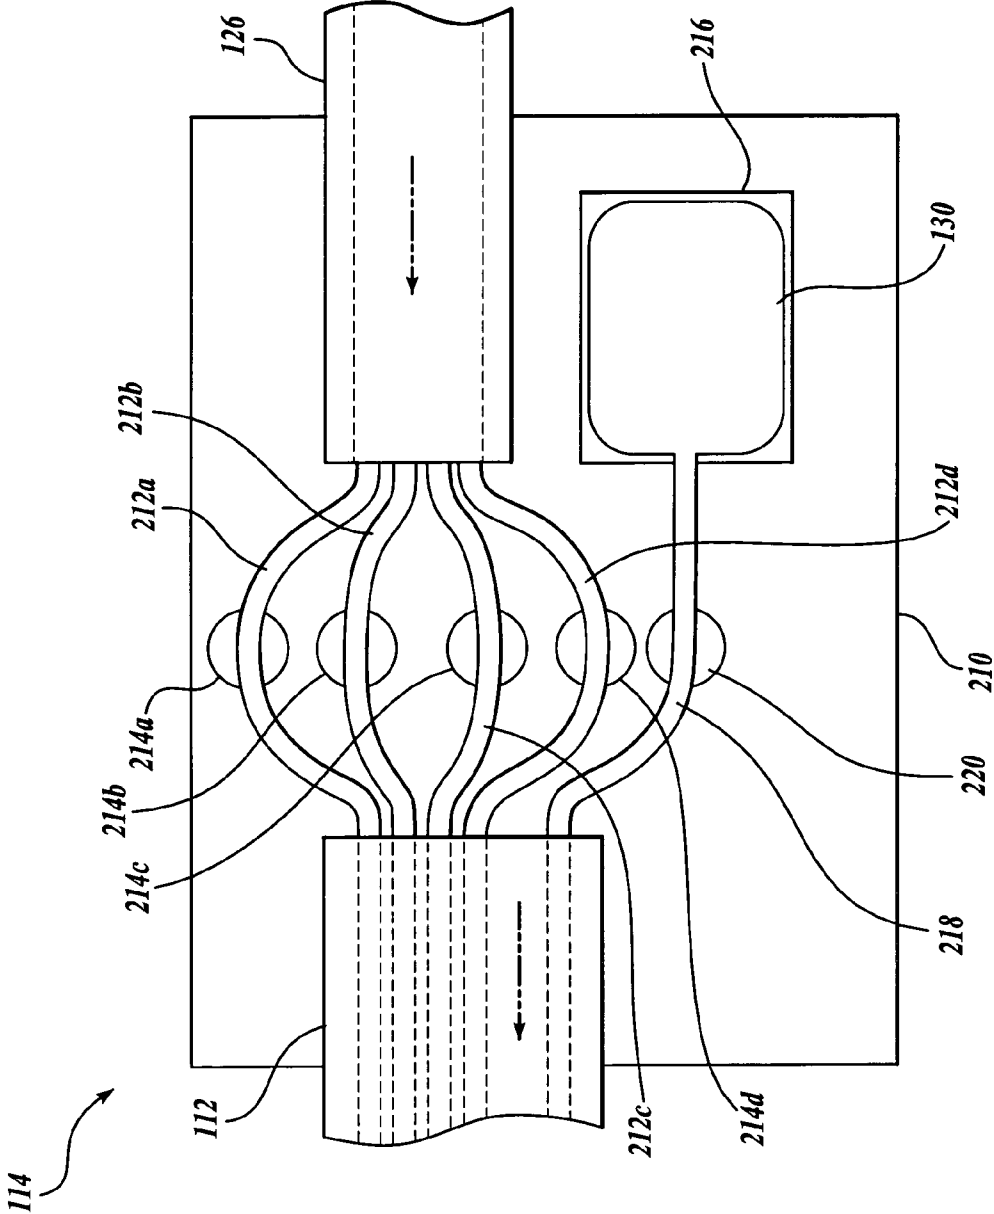


Fig. 2.



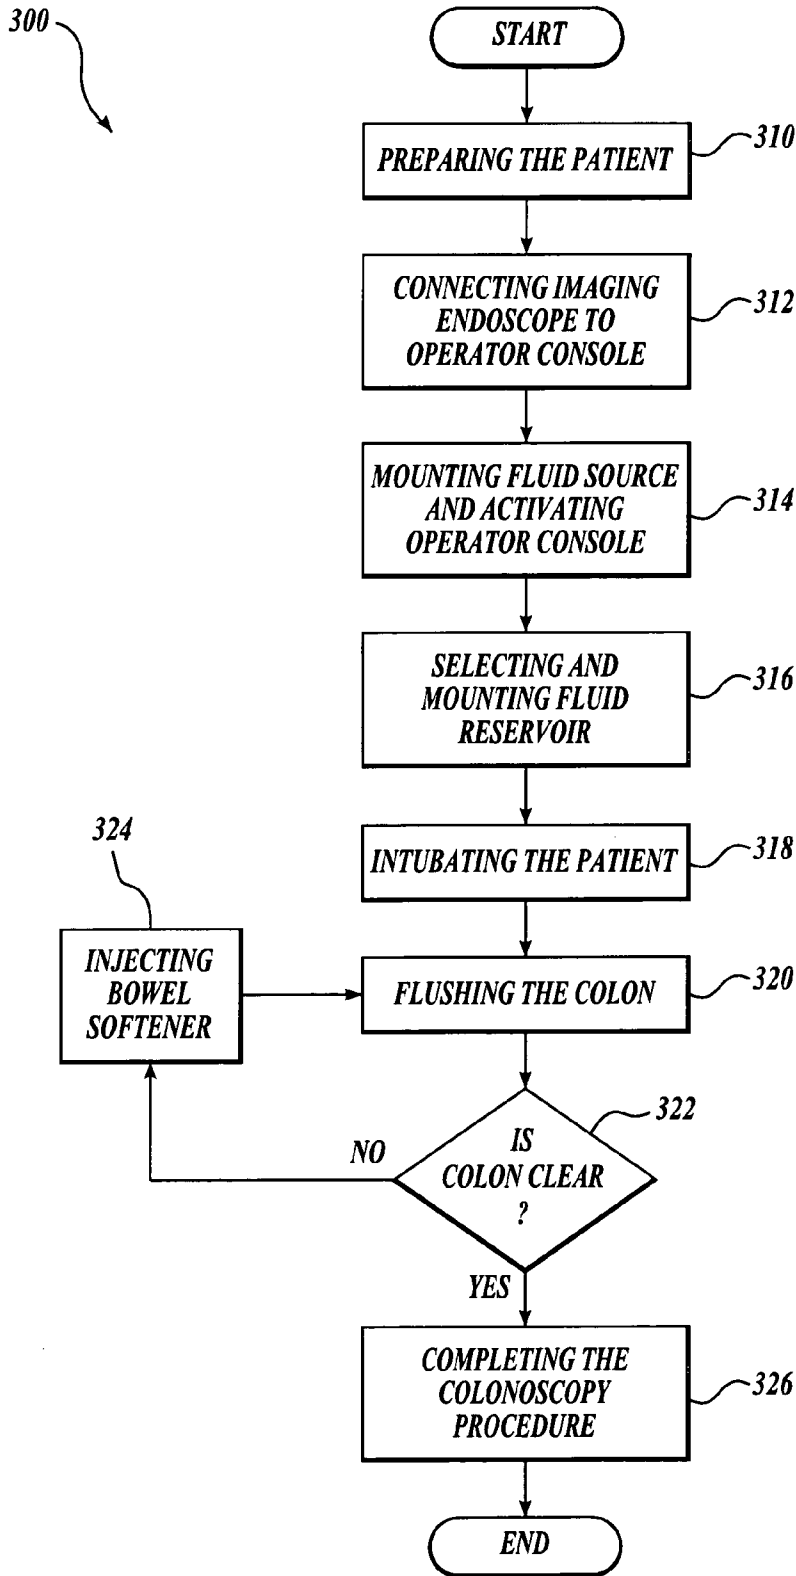

*Fig. 3.*

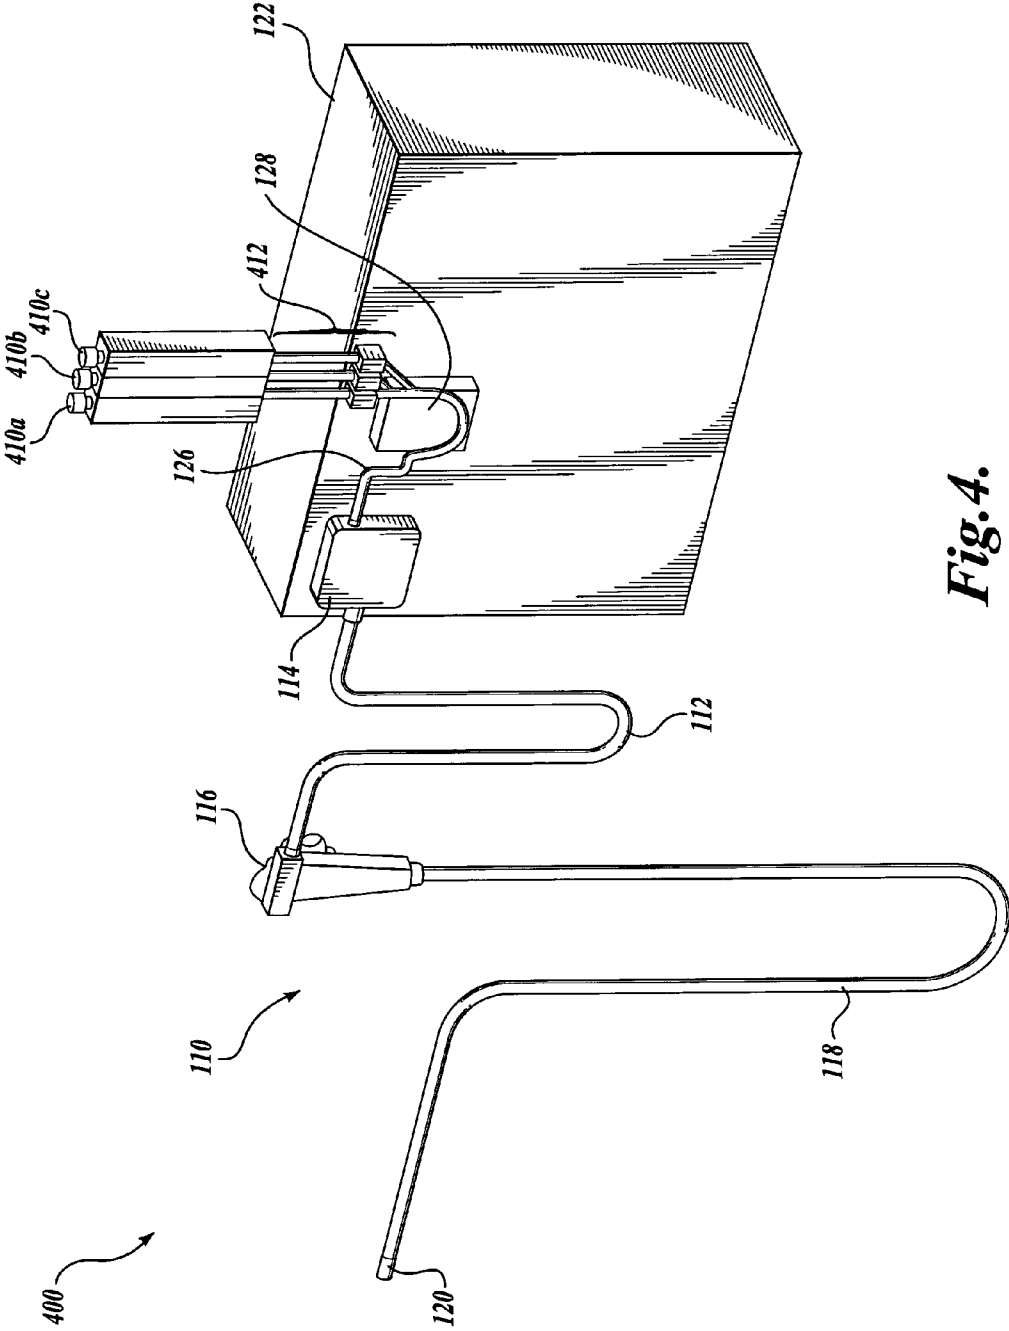


Fig.4.


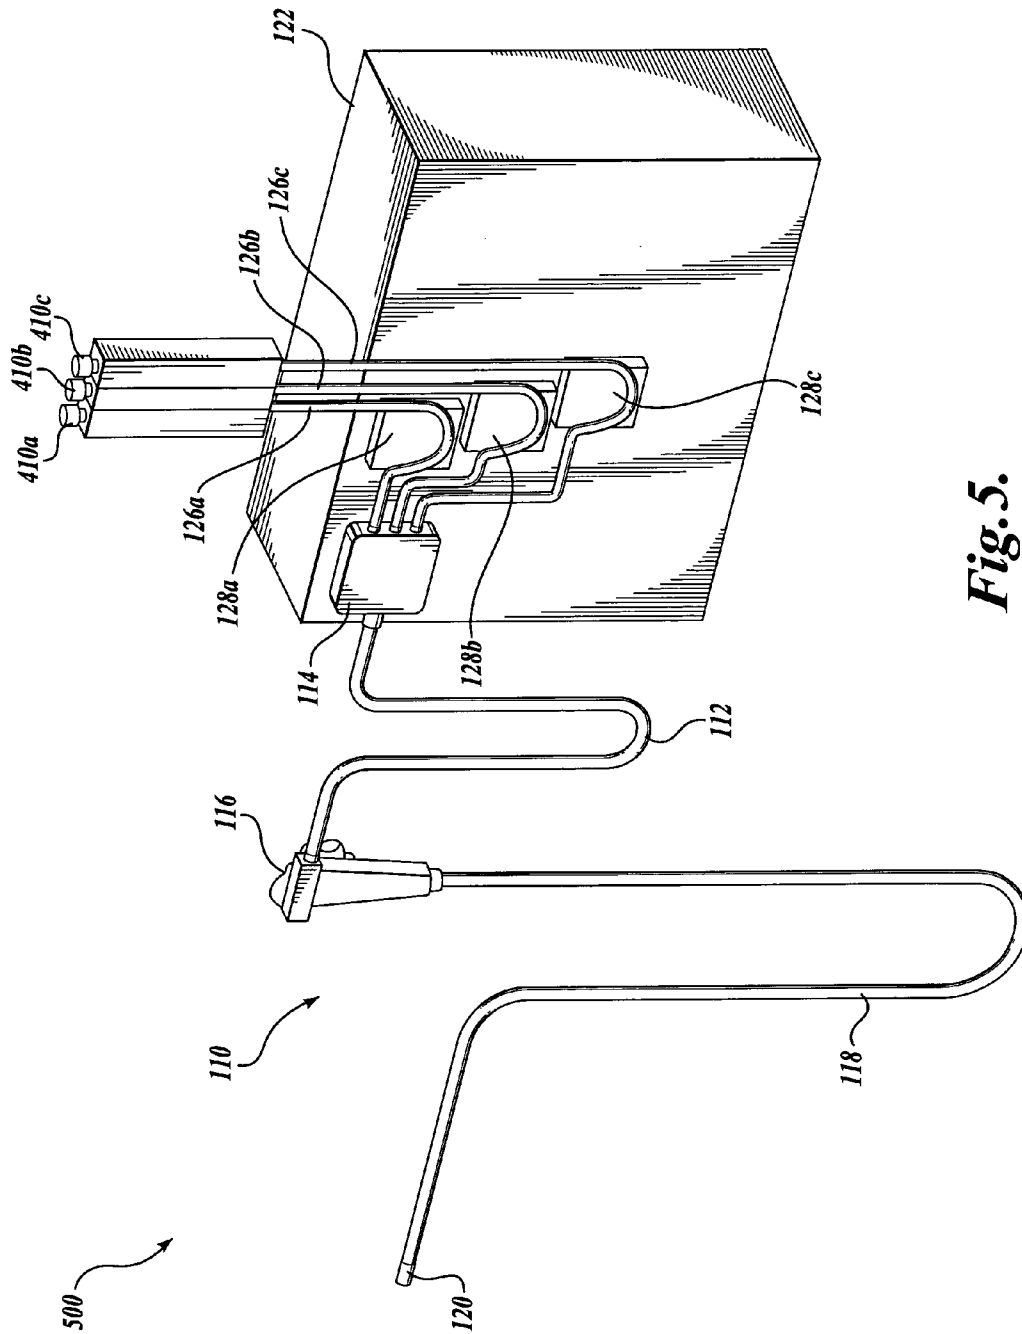


Fig. 5.

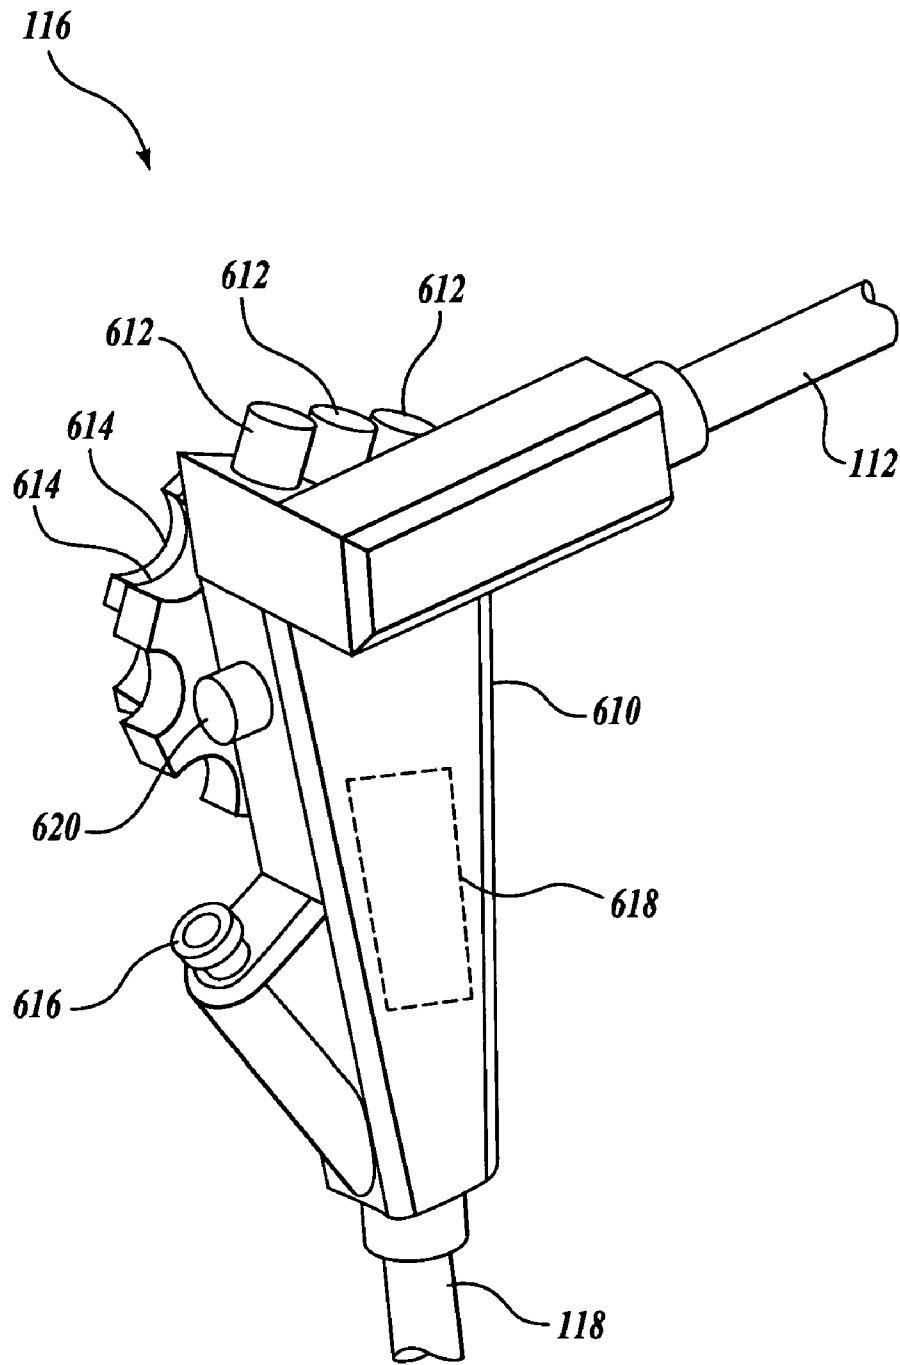

*Fig. 6.*



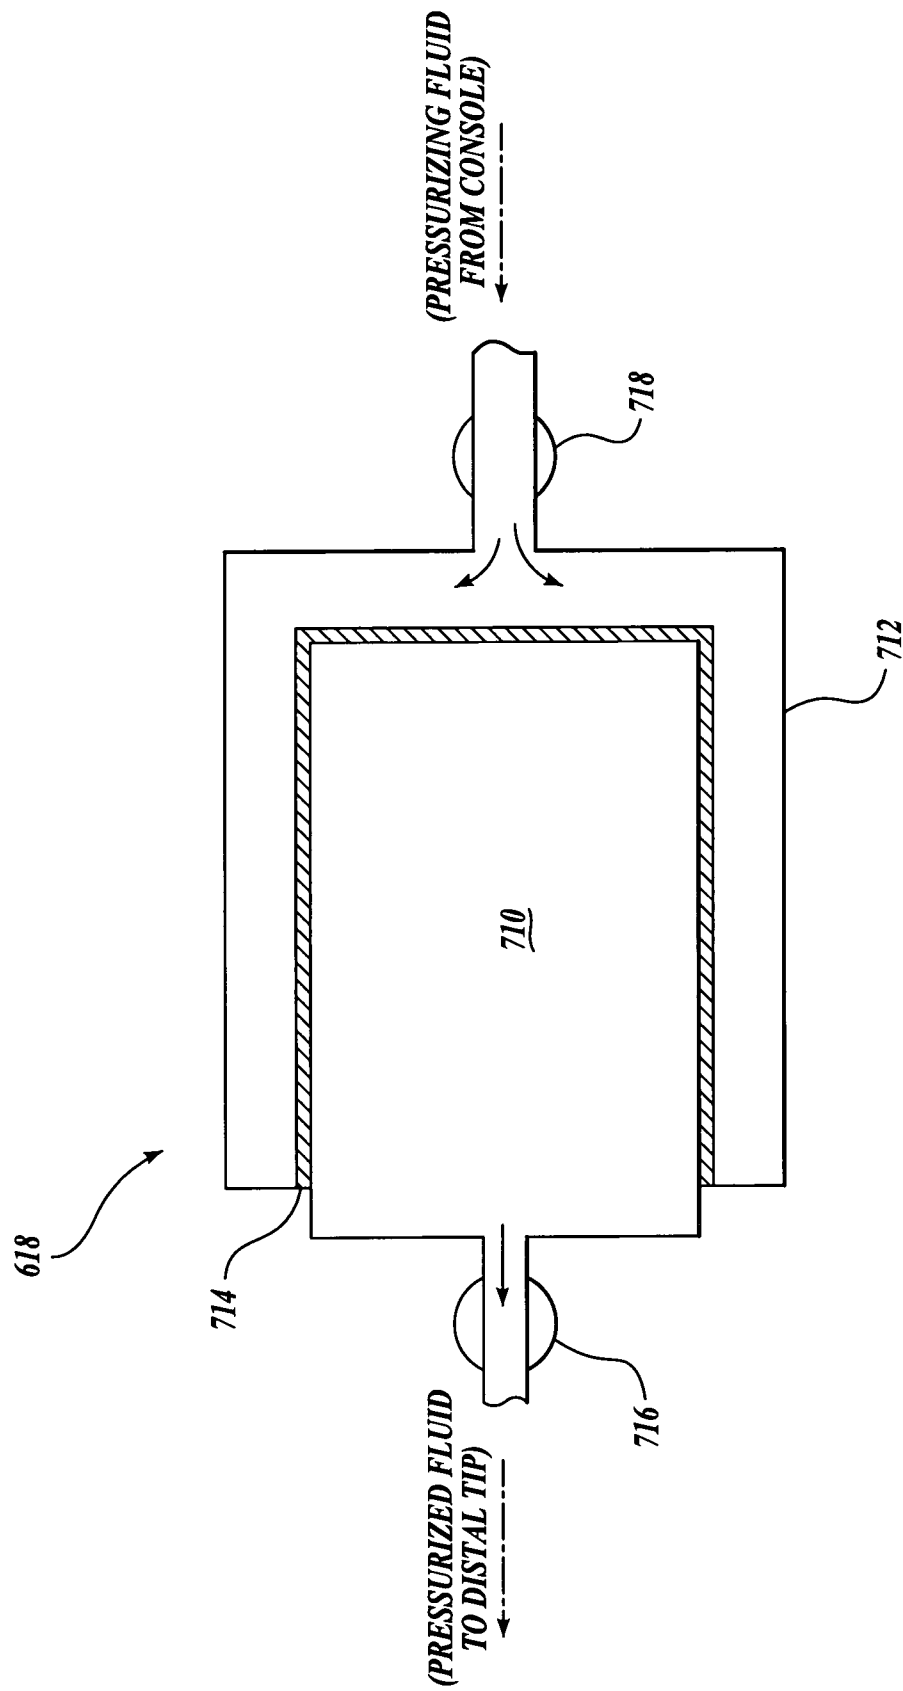



Fig. 7.

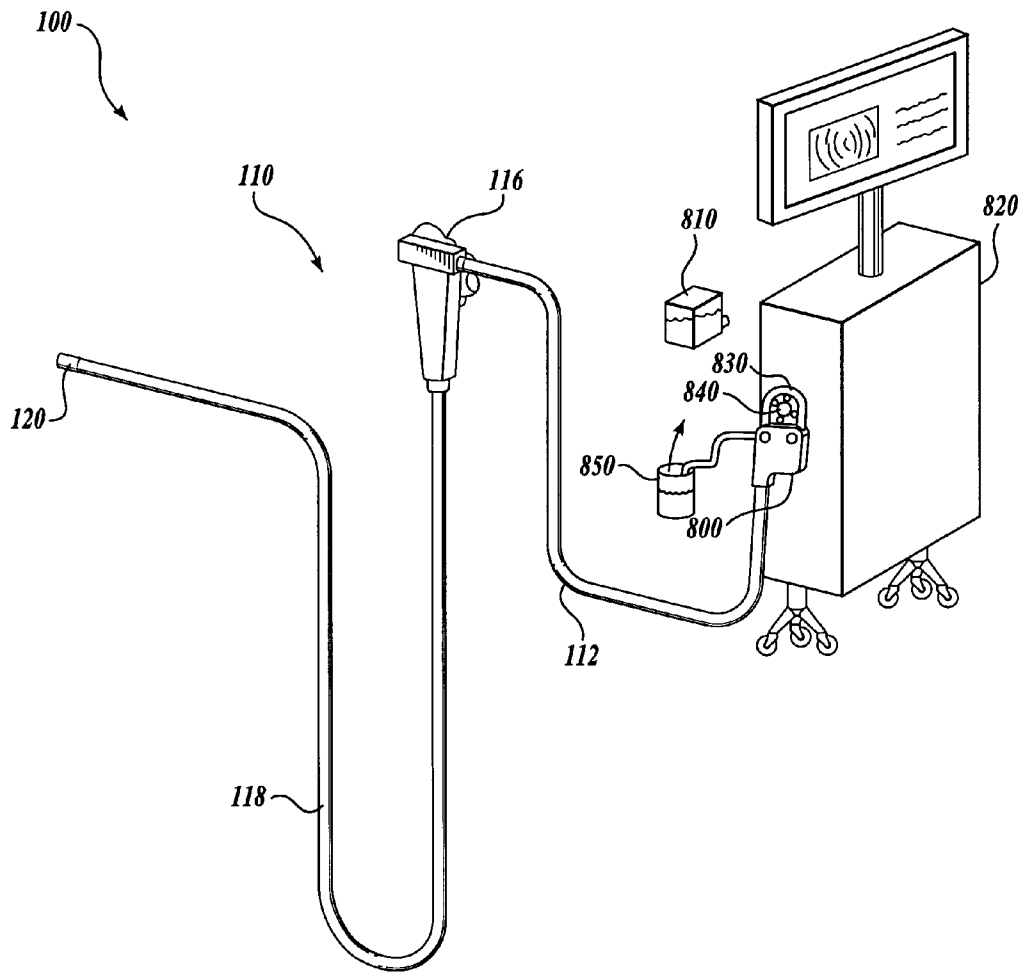

**Fig. 8.**

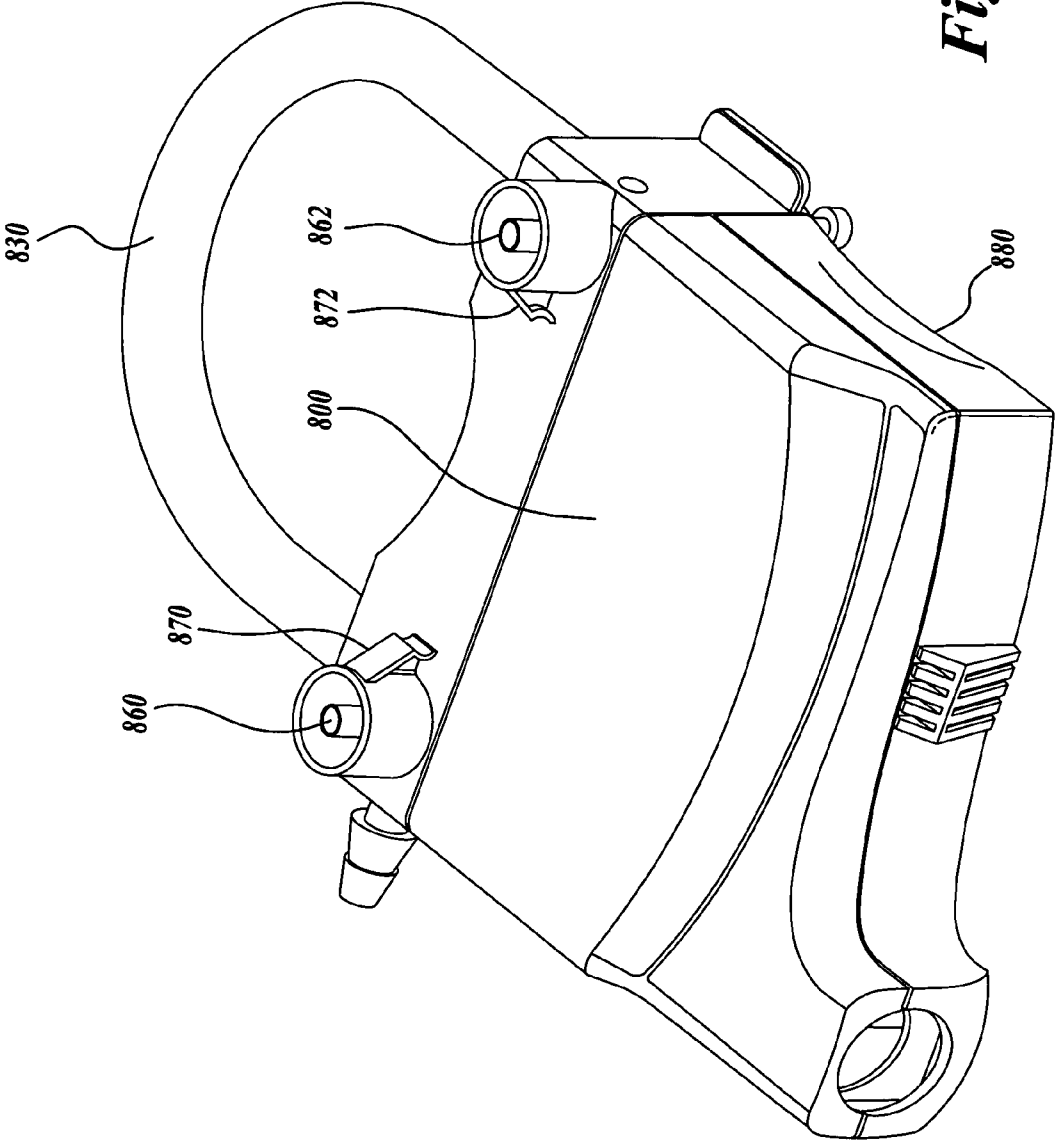


**Fig. 9A.**

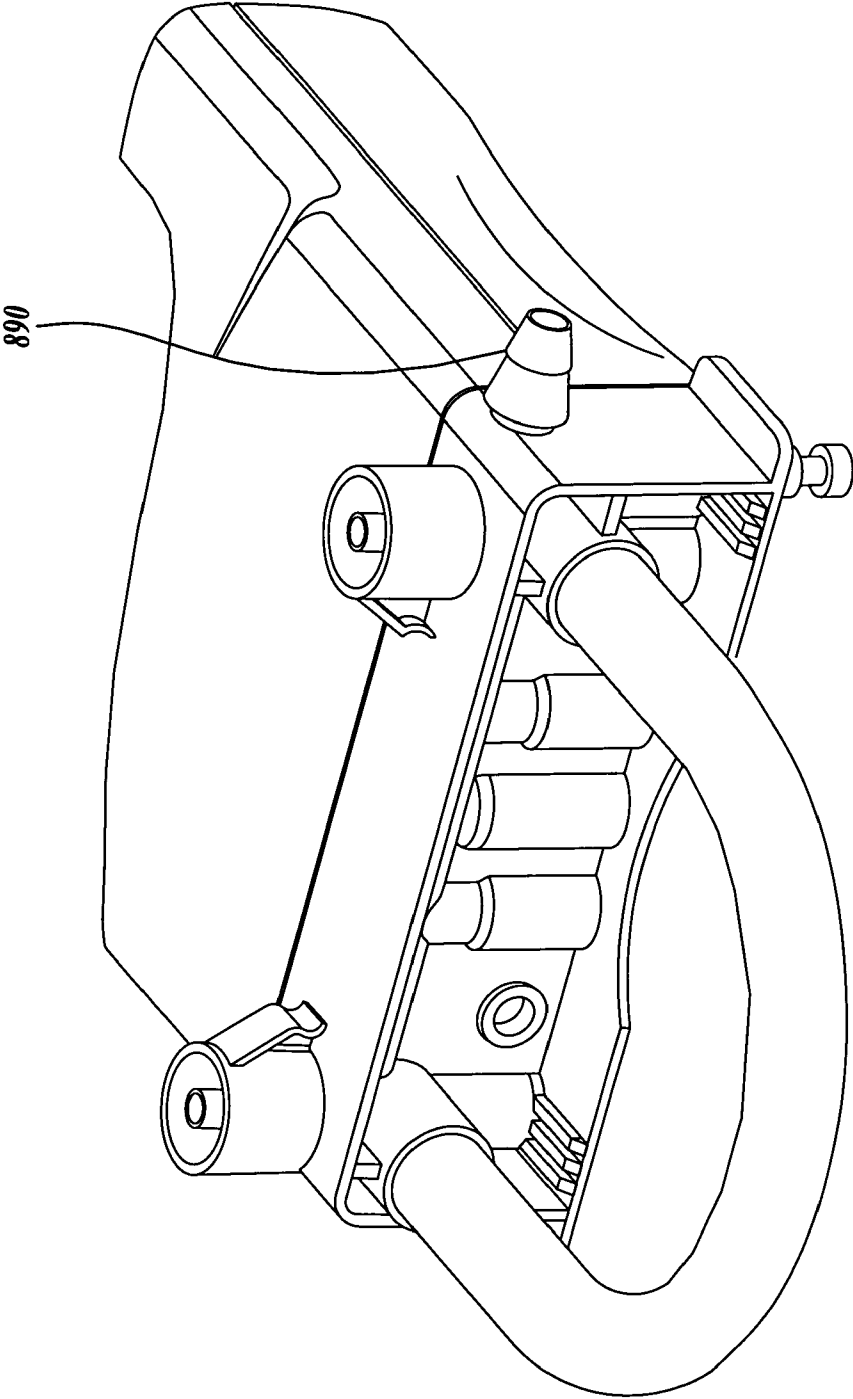


*Fig. 9B.*




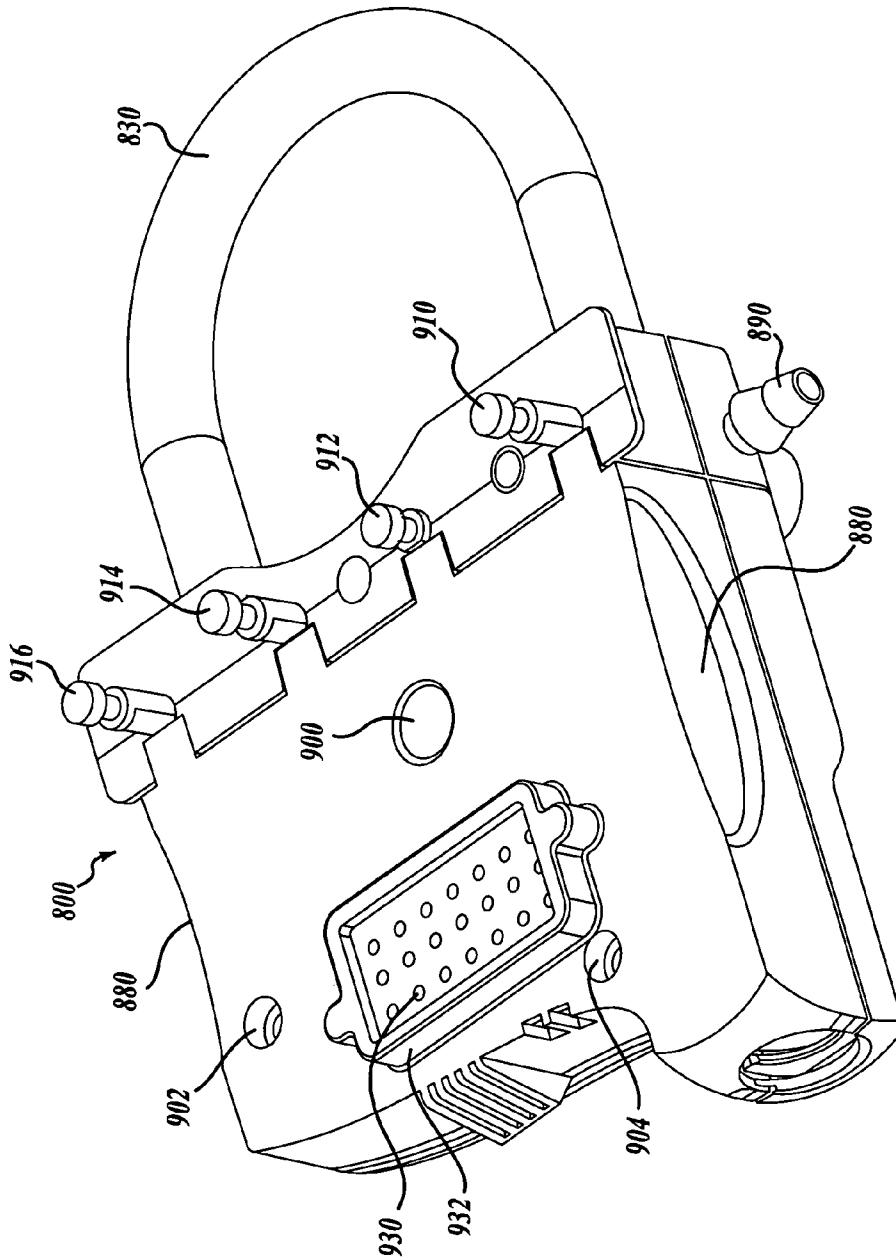


*Fig. 9C.*

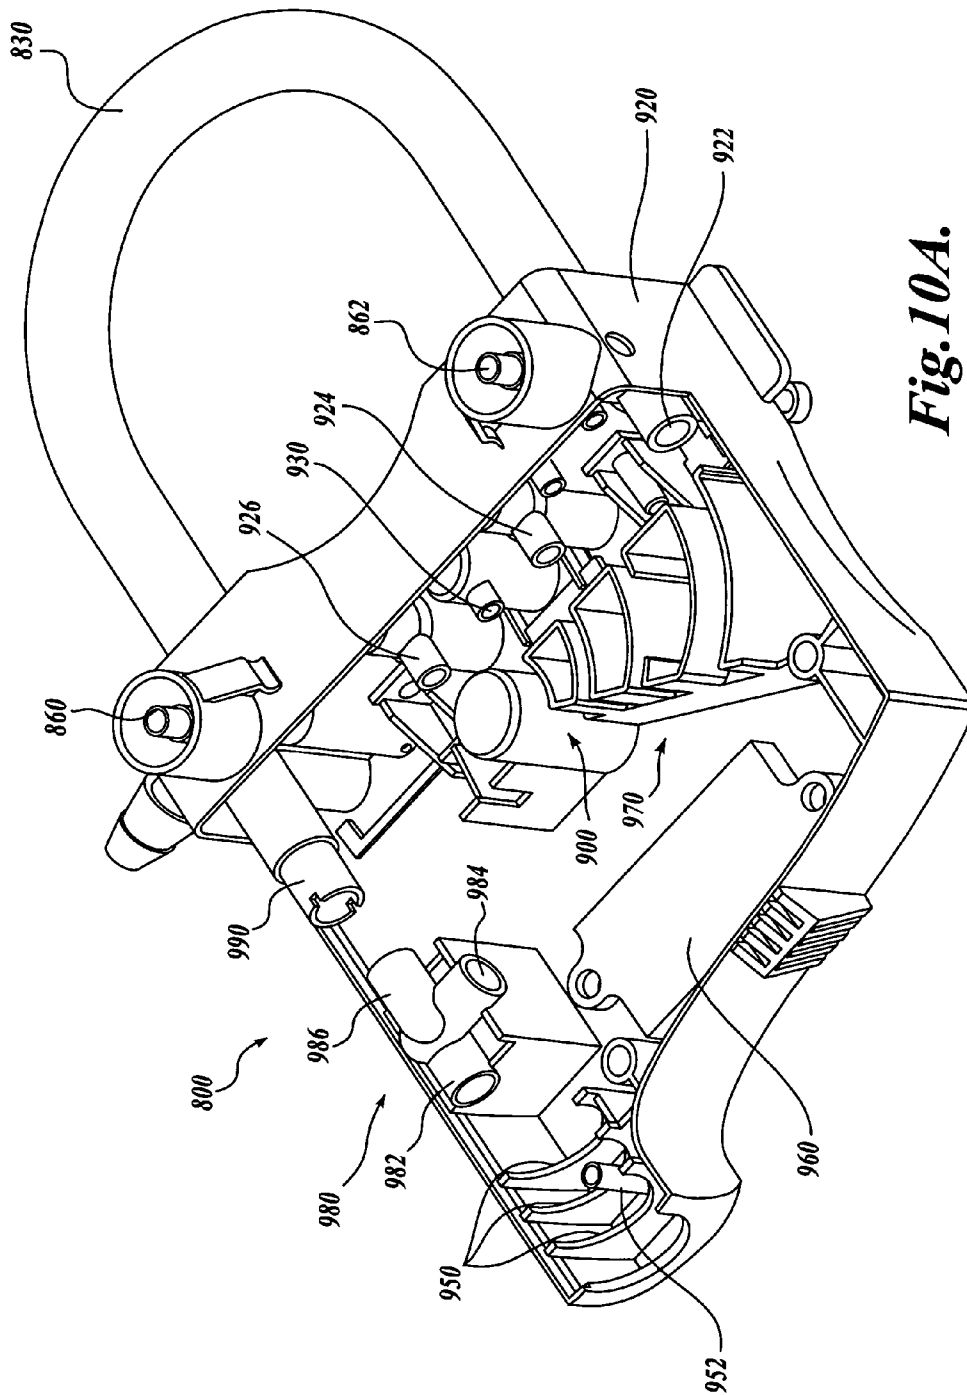


**Fig. 10A.**

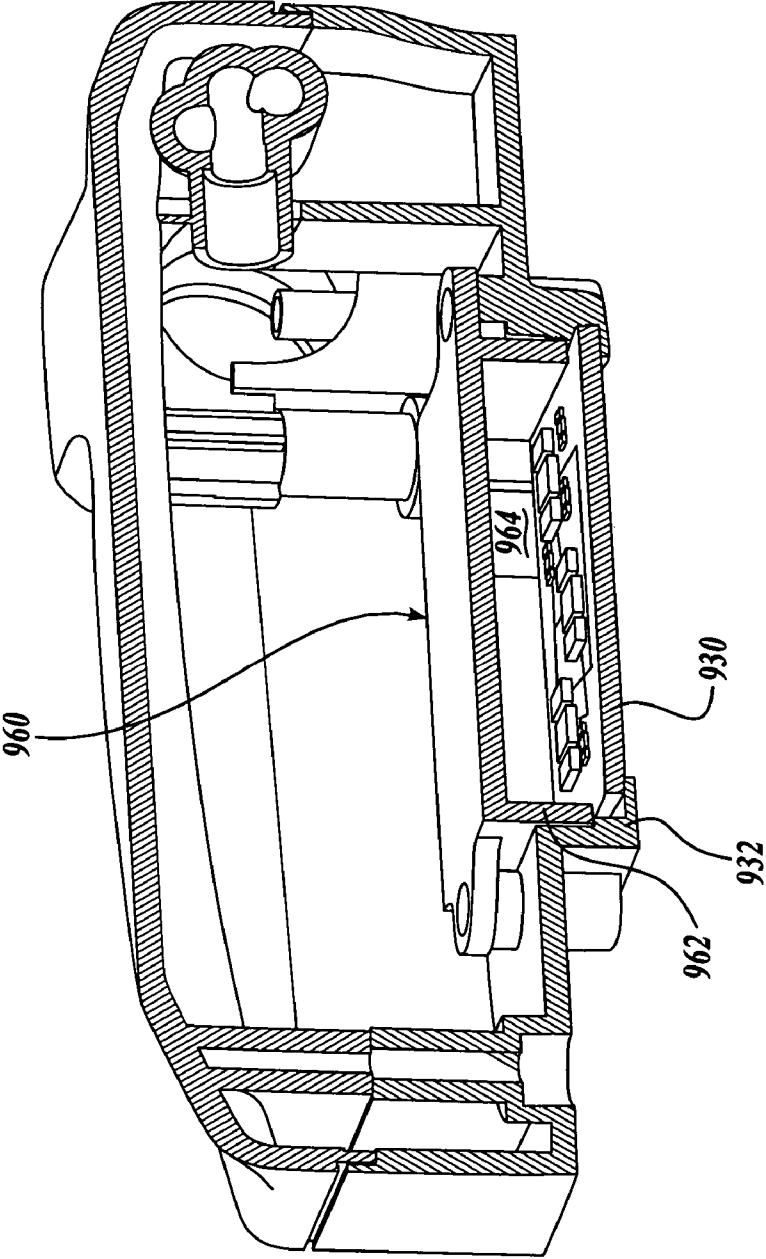


*Fig. 10B.*

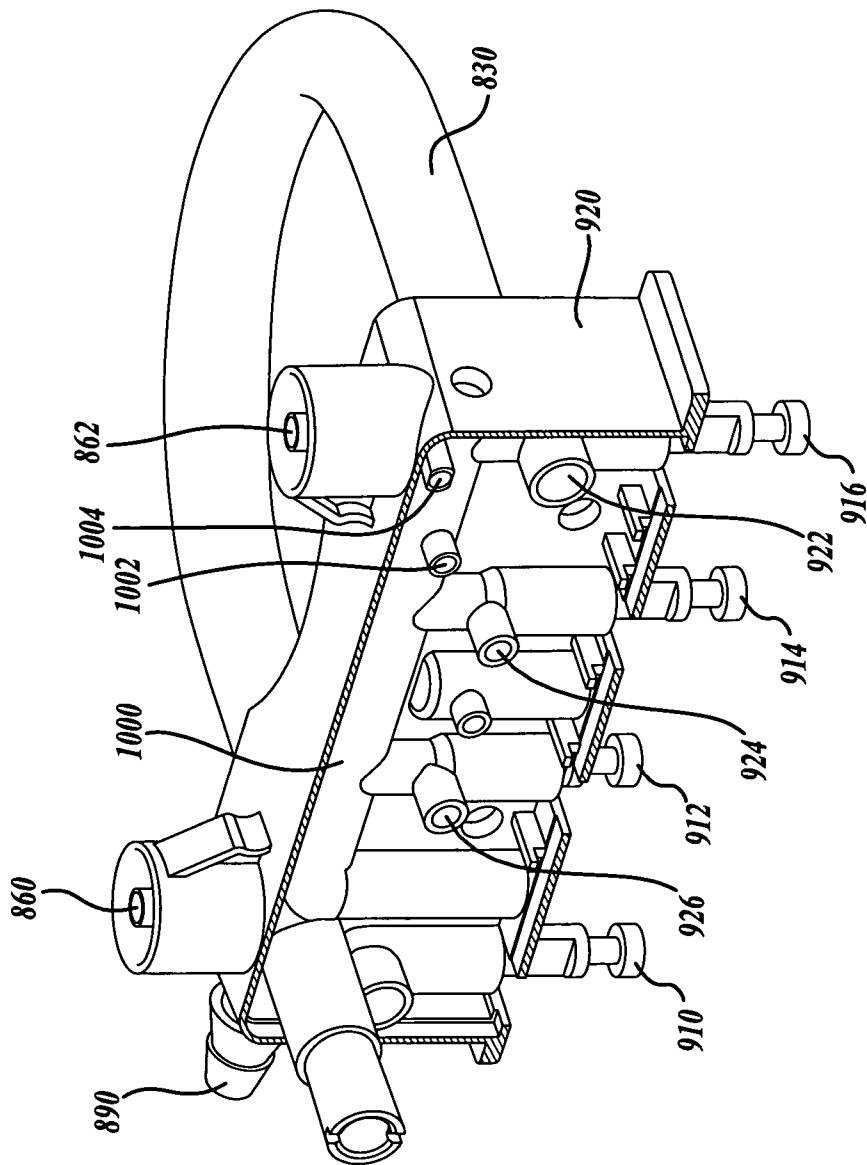


*Fig. 11A.*

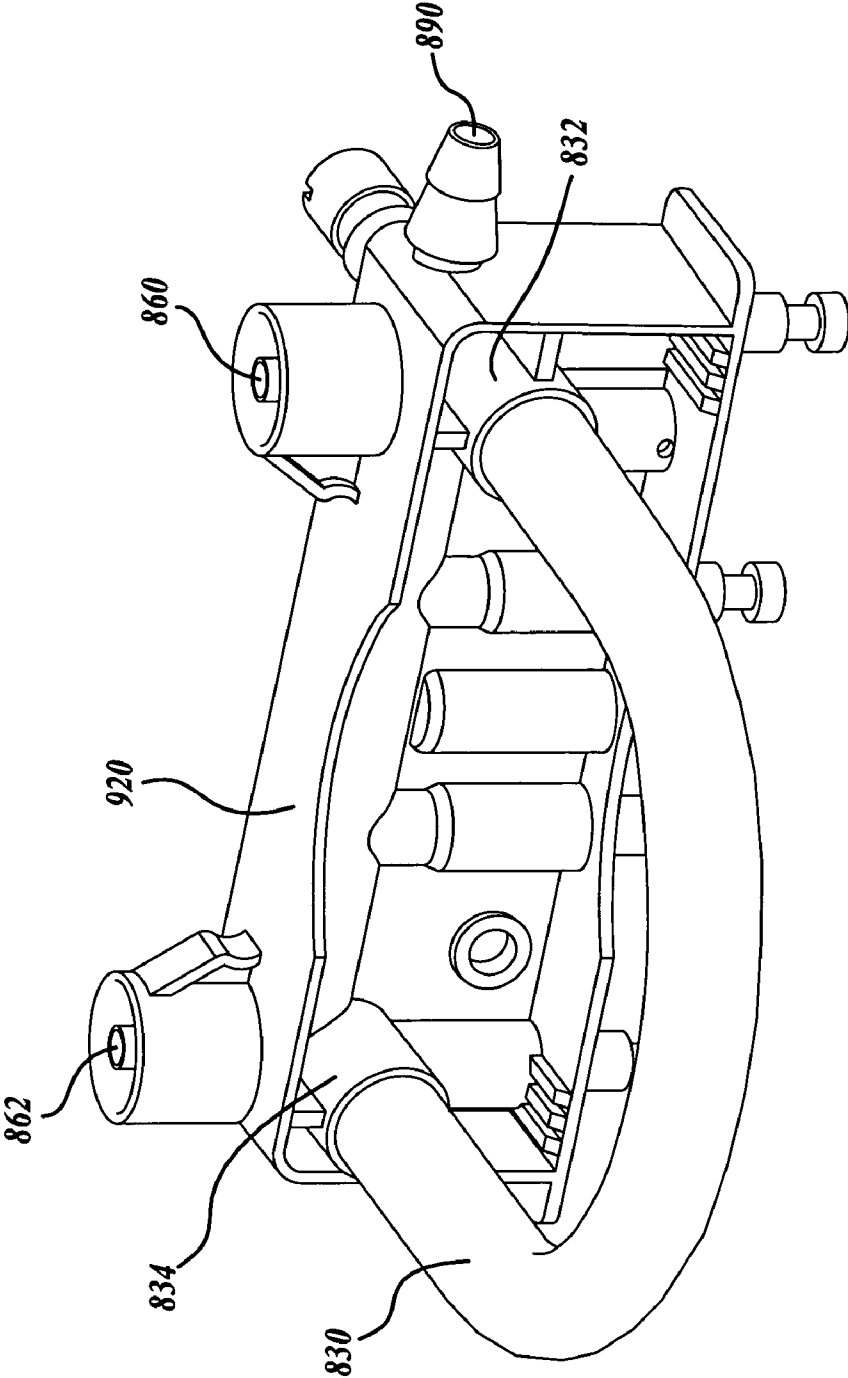


**Fig. 11B.**

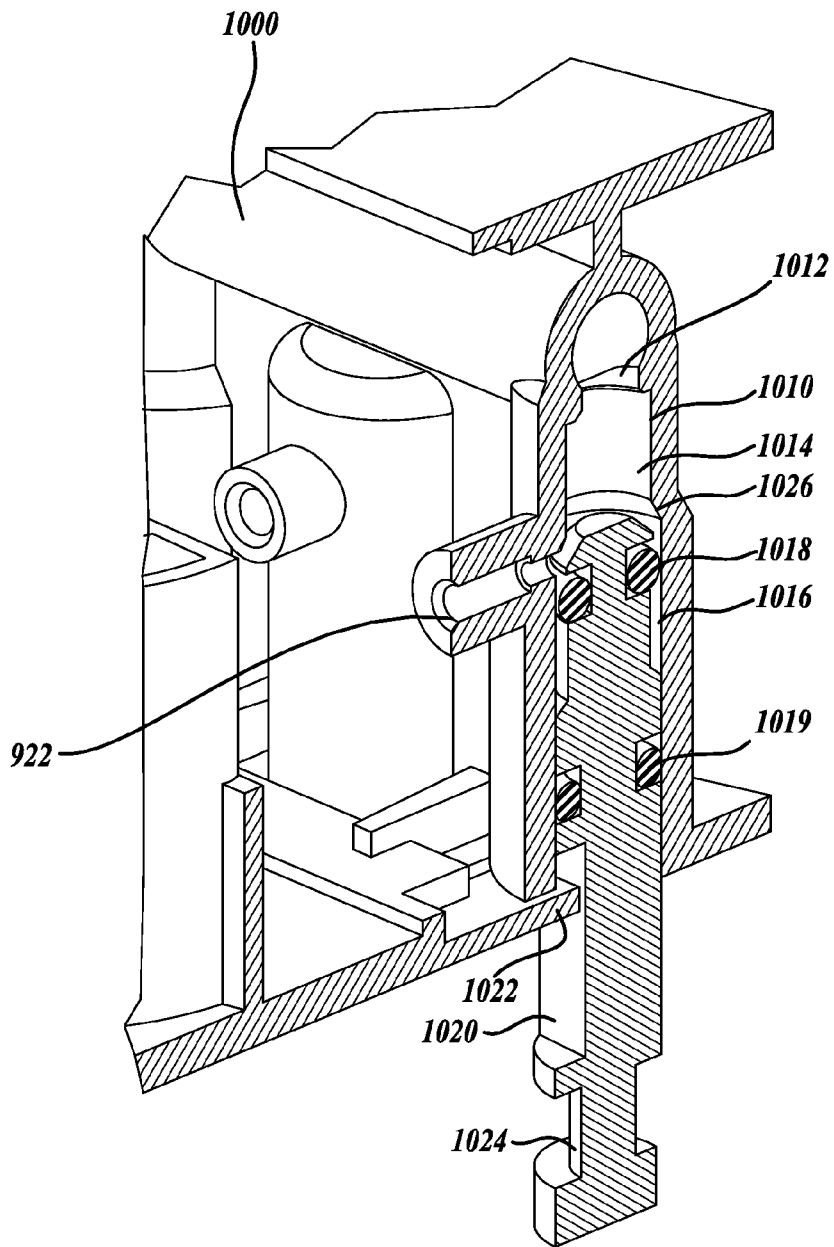

**Fig.12.**

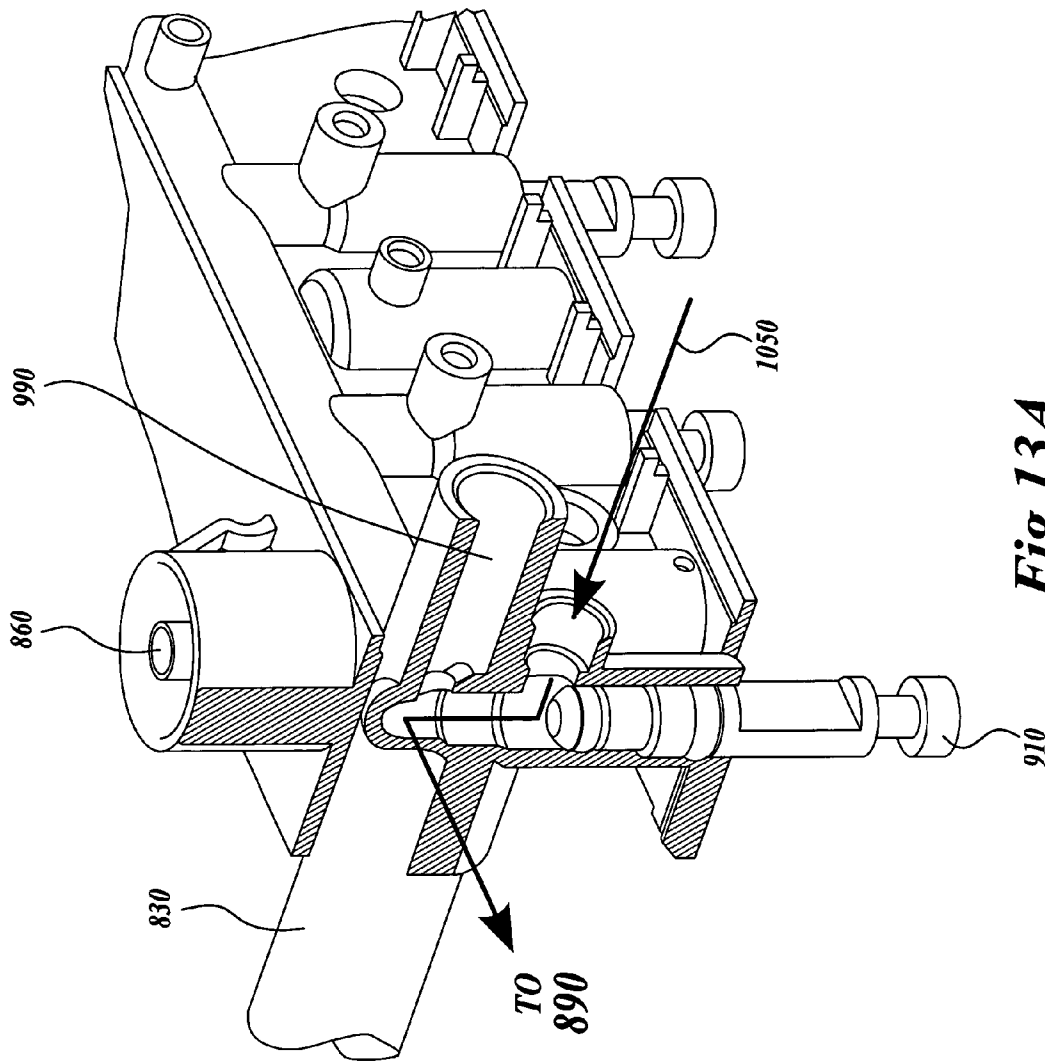


**Fig. 13A.**

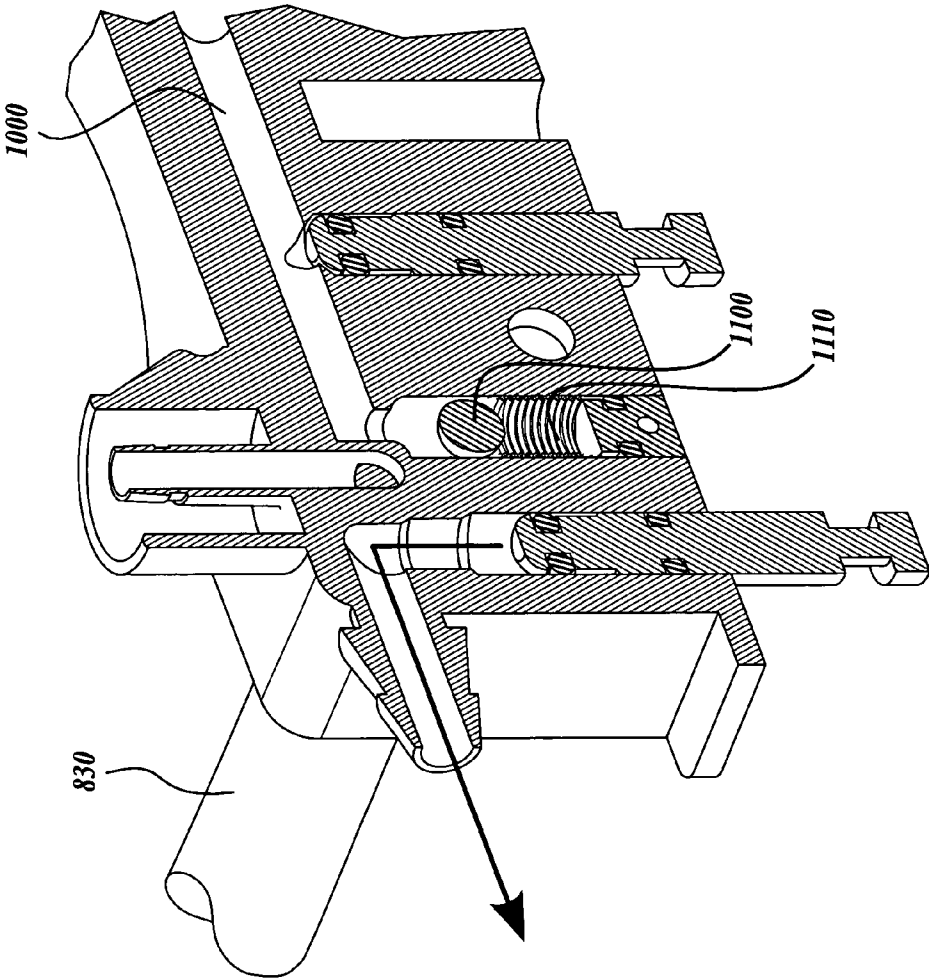

*Fig. 13B.*



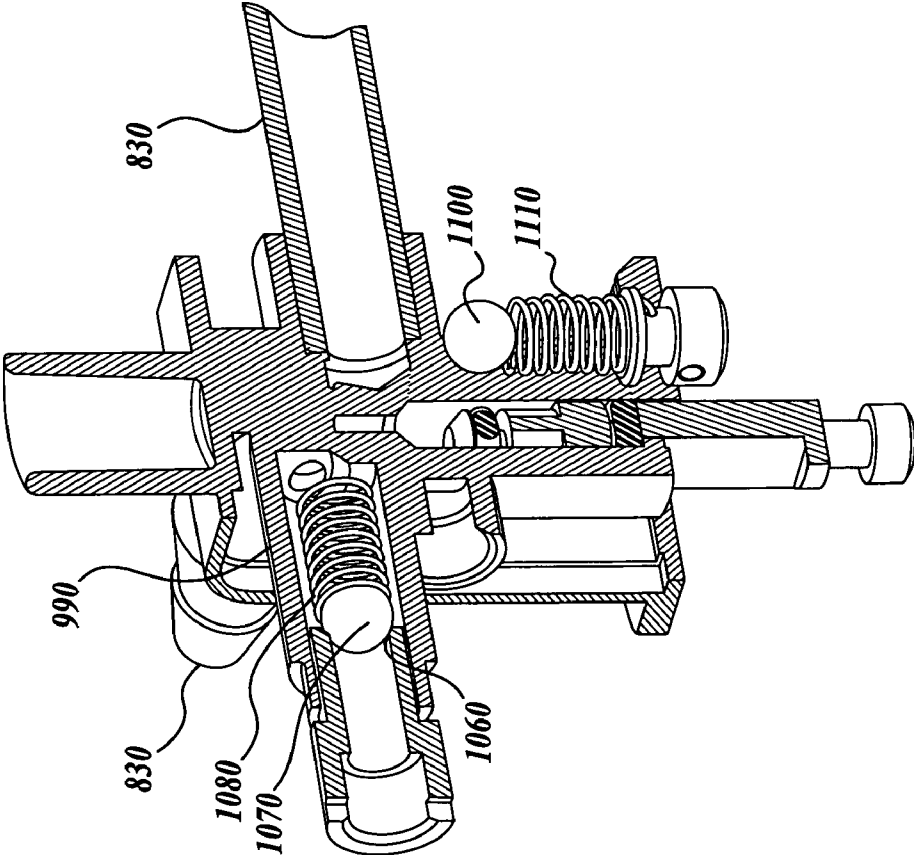

*Fig. 14.*

## FLUID DELIVERY SYSTEM FOR USE WITH AN ENDOSCOPE

### CROSS-REFERENCE TO RELATED APPLICATION

The present application claims the benefit of U.S. Provisional Application No. 60/614,868, filed Sep. 30, 2004.

### FIELD OF THE INVENTION

The present invention relates to medical devices, in general, and fluid delivery mechanisms for therapeutic and diagnostic endoscopes, in particular.

### BACKGROUND OF THE INVENTION

As an aid to the early detection of disease, it has become well established that there are major public health benefits that result from regular endoscopic examination of internal structures, such as the alimentary canals and airways, e.g., the esophagus, stomach, lungs, colon, uterus, kidney, and other organ systems. A conventional imaging endoscope used for such procedures is formed of a flexible tube that has a fiber optic light guide that directs illuminating light from an external light source to the distal tip, where it exits the endoscope and illuminates the tissue to be examined. Frequently, additional optical components are incorporated, in order to adjust the spread of light exiting the fiber bundle at the distal tip. An objective lens and fiber optic imaging light guide communicating with a camera at the proximal end of the endoscope or an imaging camera chip installed at the distal tip produces an image that is displayed to the examiner. In addition, most endoscopes include one or more working channels, through which medical devices, such as biopsy forceps, snares, fulguration probes, and other tools, may be passed.

Navigating the endoscope through complex and tortuous paths in a way that produces minimum pain, side effects, risk, or sedation to the patient is critical to the success of the examination. To this end, modern endoscopes include means for deflecting the distal tip of the endoscope to follow the pathway of the structure under examination, with minimum deflection or friction force upon the surrounding tissue. By manipulating a set of control knobs, the examiner is able to steer the endoscope during insertion and direct it to a region of interest, in spite of the limitations of such traditional control systems, which may be clumsy, non-intuitive, and friction-limited.

In any endoscopic procedure, there is almost always a need for the introduction and evacuation of different types of fluids, such as water, saline, drugs, contrast material, dyes, or emulsifiers. For example, one endoscopic procedure is a colonoscopy, which is an internal examination of the colon by means of an instrument called a colonoscope. In colonoscopy procedures, typically, 5-10% of patients who arrive for the procedure are inadequately prepared (i.e., the colon is not properly cleared) and are, therefore, turned away. Some patients who are only marginally unprepared can be fully prepared by a physician or their assistant administering doses of liquid and aspirating the colon. However, these procedures are made more difficult and time consuming because it requires the physician to flush and evacuate stool or other debris, which represents a loss of productivity.

Another endoscopic procedure is an esophagogastroduodenoscopy (EGD), which is an examination of the lining of the esophagus, stomach, and upper duodenum by means of an endoscope that is inserted down the throat. Dur-

ing an EGD procedure, the mixing of bile and water creates a lot of captivating bubbles. These bubbles hinder the physician's visibility during the procedure. As a result, a liquid is often introduced to help reduce the bubbles and, thus, improve visibility.

Yet another endoscopic procedure is an endoscopic retrograde cholangiopancreatography (ERCP), which is an endoscopic procedure used to identify stones, tumors, or narrowing in the bile ducts. In an ERCP procedure, fluids are used to flush away bleeding from sites. In addition, it is sometimes helpful to introduce dyes for providing contrast to the site. Contrast material, or contrast dye, is a substance used to make specific organs, blood vessels, or types of tissue (such as tumors) more visible on X-rays. Common contrast material substances include iodine, barium, and gadolinium.

Conventional endoscopes allow the introduction of liquids via a separate delivery device, such as a syringe or injection catheter that is passed through its working channel, in order to deliver the liquid to the distal tip of the endoscope to the target site within a patient's body. This liquid delivery method involves several steps that include, for example, the user selecting a large capacity syringe (e.g., up to 100 cc), the user pouring a desired liquid into a bowl, the user drawing the liquid into the syringe, the user attaching the syringe to the working channel of the endoscope, and the user squeezing the liquid out of the syringe. This cumbersome and time-consuming process is repeated for any and all types of liquids required in any given endoscopic procedure.

To overcome these and other problems, there is a need for an endoscope having a simplified way to introduce one or more liquids, such as water, saline, drugs, contrast material, dyes, or emulsifiers, that are used in endoscopic procedures, such as a colonoscopy procedure, an EGD procedure, or an ERCP procedure, etc. The endoscopic system should have improved simplicity and ease of use, increased efficiency, and greater clinical productivity and patient throughput. Furthermore, there is a need for improved control of the delivery rate of a liquid and improved mechanisms for mixing two or more fluids. Finally, there is a need for an endoscope that can deliver one or more liquids during a procedure and be inexpensive enough to manufacture that the device can be disposable.

### SUMMARY OF THE INVENTION

The present invention is a fluid delivery system for use with an endoscope. The fluid delivery system includes an imaging endoscope that may be used in combination with multiple fluid delivery mechanisms. In one embodiment, the imaging endoscope may be designed such that it is sufficiently inexpensive to manufacture, such that it may be considered a single-use, disposable item.

Certain embodiments of the invention include a single, large fluid source and pump installed upon a reusable operator console in combination with a small, fluid reservoir and pump installed within a proximal connector of the imaging endoscope. Other embodiments of the invention include multiple fluid sources that feed a common fluid channel and that are pressurized by a common pump. Yet other embodiments of the invention include multiple fluid sources that feed dedicated fluid channels that are pressurized by dedicated pumps, respectively. Yet other embodiments of the invention include a small, fluid reservoir and pump installed within a handheld manual controller of the imaging endoscope. The multi-fluid endoscopic systems of the present invention provide the user with the flexibility of changing fluids either in advance of a procedure or on-the-fly as needed, instead of relying on fixed

fluid sources only. Furthermore, the arrangement of fluid sources, pumps and valves within the multi-fluid endoscopic systems of the present invention provide a controlled fluid delivery rate and a controlled way of mixing fluids.

In yet another embodiment of the invention, the endoscope includes a proximal connector, including a manifold that delivers a fluid to one or more lumens in the endoscope. Valve spools are selectively actuated to deliver a pressurized liquid to one or more of its lumens.

#### BRIEF DESCRIPTION OF THE DRAWINGS

The foregoing aspects and many of the attendant advantages of this invention will become more readily appreciated as the same become better understood by reference to the following detailed description, when taken in conjunction with the accompanying drawings, wherein:

FIG. 1 illustrates a perspective view of a multi-fluid endoscopic system in accordance with an embodiment of the invention;

FIG. 2 illustrates a side view of an endoscope proximal connector in accordance with an embodiment of the invention;

FIG. 3 illustrates a flow diagram of an exemplary method of using a multi-fluid endoscopic system of the present invention during a colonoscopy procedure;

FIG. 4 illustrates a perspective view of a multi-fluid endoscopic system in accordance with another embodiment of the invention;

FIG. 5 illustrates a perspective view of a multi-fluid endoscopic system in accordance with another embodiment of the invention;

FIG. 6 illustrates a perspective view of a handheld manual controller that includes a local fluid reservoir in accordance with an embodiment of the invention;

FIG. 7 illustrates a top view of the integrated fluid reservoir that is installed, optionally, within the handheld manual controller of FIG. 6 in accordance with an embodiment of the invention;

FIG. 8 illustrates a single use endoscope having a proximal connector positioned on a reusable control unit in accordance with one embodiment of the present invention;

FIGS. 9A and 9B illustrate further details of a proximal connector;

FIG. 9C illustrates a rear surface of a proximal connector in accordance with an embodiment of the present invention;

FIG. 10A is a cutaway view of the proximal connector in accordance with an embodiment of the present invention;

FIG. 10B illustrates a circuit board retaining feature of the proximal connector in accordance with an embodiment of the present invention;

FIGS. 11A and 11B illustrate a manifold within the proximal connector in accordance with an embodiment of the present invention;

FIG. 12 illustrates a valve spool within a manifold in accordance with an embodiment of the present invention;

FIGS. 13A and 13B illustrate a vacuum line and valve within a manifold in accordance with an embodiment of the present invention; and

FIG. 14 illustrates a pressure relief valve within a manifold in accordance with an embodiment of the present invention.

#### DETAILED DESCRIPTION

FIG. 1 illustrates a perspective view of an endoscopic system 100 in accordance with a first embodiment of the invention. The endoscopic system 100 includes an imaging endo-

scope 110 that further includes an endoscope proximal shaft 112 that is electrically, mechanically, and fluidly connected, at one end, to an endoscope proximal connector 114 and, at an opposite end, to a port of a handheld manual controller 116, and an endoscope distal shaft 118 that is electrically, mechanically, and fluidly connected, at one end, to another port of handheld manual controller 116 and that has an endoscope distal tip 120 located at its opposite end for advancing into a patient's body.

Imaging endoscope 110 is an instrument that allows for the examination of the interior of a tract, lumen or vessel or hollow organ of a patient. Imaging endoscope 110 further includes an illumination mechanism (not shown), an image sensor (not shown), and an elongate shaft that has one or more lumens located therein. Imaging endoscope 110 may be sufficiently inexpensive to manufacture, such that it is considered a single-use, disposable item, such as is described in reference to U.S. patent application Ser. No. 10/406,149 filed Apr. 1, 2003, Ser. No. 10/811,781, filed Mar. 29, 2004, and Ser. No. 10/956,007, filed Sep. 30, 2004, all assigned to Scimed Life Systems, Inc./Boston Scientific Scimed, Inc., which are incorporated herein by reference. The referenced patent applications describe an endoscope imaging system that includes a reusable control cabinet that has a number of actuators or a manually operated handle on the endoscope that controls the orientation of an endoscope that is connectable thereto. The endoscope is used with a single patient and is then disposed. The endoscope includes an illumination mechanism, an image sensor, and an elongate shaft that has one or more lumens located therein. An articulation joint at the distal end of the endoscope allows the distal end to be oriented by the actuators in the control cabinet or by manual control.

The endoscopic system 100 further includes an operator console 122 that is electrically connected to standard I/O devices, such as a video display (not shown) and a keyboard (not shown). A fluid source 124 is fluidly connected to the endoscope proximal connector 114 of imaging endoscope 110 via a length of tubing 126 that passes through a pump 128. Fluid source 124 serves as a reservoir that contains a supply of liquid, such as water or saline, for use during a medical procedure. Fluid source 124 may take the form of a rigid vessel or a bladder with a capacity of, for example, up to one liter of fluid. Fluid source 124 may be a refillable vessel, or alternatively, fluid source 124 is sufficiently inexpensive to manufacture, such that it is considered a single-use, disposable item. Tubing 126 is a length of any standard flexible tubing, for example, 1/4-inch tubing, which is also sufficiently inexpensive to manufacture, such that it is considered a single-use, disposable item. Pump 128 is, for example, a standard peristaltic pump, that is used to withdraw liquid from fluid source 124 on demand. A peristaltic pump works by means of rollers on rotating arms that pinch the flexible tubing against an arc and, thus, move the fluid along. Pump 128 is capable of delivering, for example, up to 50 pounds/square inch (PSI) of pressure for a flow rate of, for example, 500 ml/min.

In one embodiment, the endoscope proximal connector 114 of imaging endoscope 110 is electrically and mechanically connected to the exterior of operator console 122, as shown in FIG. 1, via a quick-release mechanism for making and breaking all electrical, mechanical, and fluid/air/vacuum connections. The quick-release mechanism allows endoscope proximal connector 114 to be secured easily to the exterior of operator console 122. Endoscope proximal connector 114 includes wires and tubes that pass through endoscope proximal shaft 112, then through a handheld manual

controller 116, then through endoscope distal shaft 118, and then to endoscope distal tip 120. Additionally, mounted within endoscope proximal connector 114 is a fluid reservoir 130 that has an associated pump (not shown) mounted within operator console 122. Endoscope proximal connector 114 and fluid reservoir 130 are described in more detail in reference to FIG. 2.

Endoscope proximal shaft 112 and endoscope distal shaft 118 are formed of a suitably lightweight, flexible material, such as polyurethane or other biocompatible materials. Endoscope proximal shaft 112 and endoscope distal shaft 118 are elongated shafts that have one or more lumens located therein and wiring located therein to support, for example, a working channel, a jet wash mechanism, an illumination mechanism, and an image sensor that are located at endoscope distal tip 120. Also included within handheld manual controller 116 and endoscope distal shaft 118 are the electrical and mechanical mechanisms for articulating endoscope distal tip 120 for advancing into a patient.

Handheld manual controller 116 of imaging endoscope 110 is a handheld device that is electrically and mechanically connected to operator console 122. Handheld manual controller 116 accepts inputs from a human operator via standard push buttons, rotary knobs, joysticks, or other activation devices, either singularly or in combination, to control the operation of imaging endoscope 110, which includes the delivery of pressurized liquid from fluid source 124. Alternatively, a user input device such as a keyboard or other user interface located remotely from the endoscope may accept inputs from a human operator to control the operation of the imaging endoscope 110, including the delivery of pressurized liquid from fluid source 124.

Operator console 122 is a special-purpose electronic and electromechanical apparatus that facilitates, processes, and manages all functions of multi-fluid endoscopic system 100. Operator console 122 is loaded with software for managing, for example, the operation of imaging endoscope 110 and its associated imaging electronics (not shown) in order to create and/or transfer images received from an image sensor within imaging endoscope 110 to the video display for viewing by a user. Operator console 122 further manages the operation of all pumps, such as pump 128.

FIG. 2 illustrates a side view of an exemplary endoscope proximal connector 114 in accordance with an embodiment of the present invention. Endoscope proximal connector 114 includes a proximal connector housing 210 that is formed of a suitably lightweight, rigid material, such as molded plastic. An end of tubing 126, which is a single fluid channel, is split into an arrangement of multiple fluid channels 212, for example, a fluid channel 212a, 212b, 212c, and 212d. Fluid channels 212a, 212b, 212c, and 212d are fed separately into and along the full length of endoscope proximal shaft 112 to endoscope distal tip 120.

Fluid channels 212a, 212b, 212c, and 212d are used, for example, for supplying fluid, such as water, from fluid source 124 via pump 128 for (1) cooling light-emitting diodes (LEDs) (i.e., the illumination mechanism), (2) supplying a low pressure bolus wash, (3) supplying a high pressure jet wash, and (4) supplying a lens wash, all of which are located at endoscope distal tip 120. Multiple fluid channels 212 are controlled via multiple respective pinch valves 214. More specifically, fluid channels 212a, 212b, 212c, and 212d are controlled via pinch valves 214a, 214b, 214c, and 214d, respectively. Pinch valves 214 are standard valves, within which the flexible tubing of fluid channels 212 is pinched between one or more moving external elements, in order to stop the flow of fluid.

FIG. 2 also shows fluid reservoir 130 fitted into a recessed cavity 216 within endoscope proximal connector 114. Fluid reservoir 130 is fluidly connected to a fluid channel 218 that is fed into and along the full length of endoscope proximal shaft 112 and delivers the fluid from fluid reservoir 130 to endoscope distal tip 120. The flow of fluid is controlled by a pinch valve 220 that is identical to pinch valves 214. Fluid reservoir 130 is in the form of, for example, a disposable, soft, flexible bag or bladder that is easily detachable from fluid channel 218. The capacity of liquid held within fluid reservoir 130 is relatively small, compared with the capacity of fluid source 124. Fluid reservoir 130 may be sized, for example, to hold a small quantity of irrigation liquids, contrast media, medication, or dyes for marking tissue. An access door (not shown) may be included within proximal connector housing 210 for installing or removing fluid reservoir 130 as needed before, after, or during a medical procedure. The liquid within fluid reservoir 130 may be pressurized with any well-known mechanisms, such as a piston (not shown) that pushes against the bladder that forms fluid reservoir 130. Additionally, electrical wires (not shown) pass through endoscope proximal connector 114 between handheld manual controller 116 and operator console 122 for controlling the flow of fluids via the combined functions of pinch valves 214a, 214b, 214c, or 214d and pump 128 and/or pinch valve 220 and the pressurizing mechanism of fluid reservoir 130.

In operation, and with continuing reference to FIGS. 1 and 2, pressurized fluids from fluid source 124 and/or fluid reservoir 130 are delivered along the full length of endoscope proximal shaft 112 to endoscope distal tip 120, on demand, under the control of electronics located within operator console 122. More specifically, pump 128 and the pressurizing mechanism of fluid reservoir 130 are activated, and the user controls the on-demand delivery of fluid, for example, to supply a low pressure bolus wash via the working channel of imaging endoscope 110, to supply a high pressure jet wash at endoscope distal tip 120, or to supply a lens wash at endoscope distal tip 120, all via push buttons on handheld manual controller 116 that control pinch valves 214a, 214b, 214c, or 214d. Additionally, the user controls the on-demand delivery of fluid from fluid reservoir 130 via a push button on handheld manual controller 116 that controls pinch valve 220 and the pressurizing mechanism (not shown) of fluid reservoir 130, for example, to deliver medication or dye through endoscope distal shaft 118 of imaging endoscope 110 and out of endoscope distal tip 120 to a tissue site within the patient. Pressurized fluids from fluid source 124 and/or fluid reservoir 130 may be delivered continuously to the endoscope distal tip 120 to supply cooling to the LEDs.

FIG. 3 illustrates a flow diagram of an exemplary method 300 of using multi-fluid endoscopic system 100 to handle a poorly prepared patient during a colonoscopy procedure in accordance with the invention. Method 300 and multi-fluid endoscopic system 100 are not limited to a colonoscopy procedure. Those skilled in the art will recognize that the method steps of method 300 may be adapted easily to apply to any of the various medical procedures that use various types of fluid sources, respectively. Method 300 includes the steps of:

#### Step 310: Preparing the Patient

In this step, in a predetermined time period prior to the time of the colonoscopy procedure, a patient consumes a quantity of, for example, a phosphosoda solution or a colyte solution, which serves as a laxative to flush stool out of the patient's colon. Alternatively, the patient arrives with no or insufficient preparation and the physician manually clears the patient's colon with a colon preparation endoscope. Method 300 proceeds to step 312.

**Step 312: Connecting Imaging Endoscope to Operator Console**

In this step, a user, which may be a physician, nurse, or other assistant, attaches endoscope proximal connector **114** of imaging endoscope **110** to the side of operator console **122** and thereby makes all electrical and fluid connections to operator console **122**. The user activates operator console **122**. Method **300** proceeds to step **314**.

**Step 314: Mounting Fluid Source and Activating Operator Console**

In this step, a user mounts fluid source **124** to operator console **122** and, subsequently, connects tubing **126**, at one end, to the outlet of fluid source **124** and, at the opposite end, to a port of endoscope proximal connector **114**, while, at the same time, passing a portion of tubing **126** within pump **128**. The user then activates operator console **122**. Method **300** proceeds to step **316**.

**Step 316: Selecting and Mounting Fluid Reservoir**

In this step, a user selects a fluid reservoir **130** that contains the type of liquid required for the medical procedure, such as a bowel softener in the case of a colonoscopy procedure and, subsequently, mounts fluid reservoir **130** within cavity **216** of endoscope proximal connector **114**. Method **300** proceeds to step **318**.

**Step 318: Intubating the Patient**

In this step, under the control of operator console **122** and by using the controls of handheld manual controller **116**, the physician intubates the patient, by introducing and advancing endoscope distal tip **120** of imaging endoscope **110** into a body cavity of the patient, until such time that the area of the colon to be cleared may be visualized upon video display of operator console **122**. Method **300** proceeds to step **320**.

**Step 320: Flushing the Colon**

In this step, under the control of operator console **122** and by using the controls of handheld manual controller **116**, the user alternately flushes and aspirates the patient's colon, by alternately activating the bolus wash and/or jet wash function and a suction function of multi-fluid endoscopic system **100**. In doing so, the user controls the activation of pump **128**, one or more pinch valves **214**, and a suction/vacuum source (not shown) via the controls of handheld manual controller **116**. Method **300** proceeds to step **322**.

**Step 322: Is Colon Clear?**

In this decision step, the user visualizes the colon by using the imaging electronics at endoscope distal tip **120**, in combination with the video display of operator console **122**, to determine whether the bolus wash and/or jet wash of step **320** is effective in breaking down the stool in the patient's colon and, thus, renders the colon clear. If yes, method **300** proceeds to step **326**. If no, method **300** proceeds to step **324**.

**Step 324: Injecting Bowel Softener**

In this step, under the control of operator console **122** and by using the controls of handheld manual controller **116**, the user injects a bowel softener to help emulsify the stool by controlling pinch valve **220**, such that the bowel softener within fluid reservoir **130** that is mounted within endoscope proximal connector **114** is released and, thus, passes into the patient's colon via fluid channel **218** of endoscope proximal shaft **112**. Method **300** returns to step **320**.

**Step 326: Completing the Colonoscopy Procedure**

In this step, under the control of operator console **122** and by using the controls of handheld manual controller **116**, the user completes the colonoscopy procedure which may include such steps as selecting another type of liquid for installing into fluid reservoir **130** within cavity **216** of endo-

scope proximal connector **114**. Such fluids include, for example, an India ink for marking a tissue site. Method **300** then ends.

FIG. 4 illustrates a perspective view of a multi-fluid endoscopic system **400** in accordance with a second embodiment of the invention. Multi-fluid endoscopic system **400** includes imaging endoscope **110** that is connected to operator console **122** via endoscope proximal connector **114**, as described in reference to FIGS. 1 and 2. Multi-fluid endoscopic system **400** includes pump **128**, as described in reference to FIG. 1. Multi-fluid endoscopic system **400** further includes a plurality of fluid sources **410**, e.g., a fluid source **410a**, **410b**, and **410c**, that feed tubing **126** via a tubing subassembly **412** that brings together the tubing from the separate fluid sources **410** to a common line, i.e., tubing **126**, and wherein each fluid source **410** has an associated pinch valve that allows liquid to reach the pump **128**. Each fluid source **410** may take the form of a rigid vessel or a bladder with a capacity of, for example, up to one liter of fluid. Each fluid source **410** may be a refillable vessel, or alternatively, each fluid source **410** is sufficiently inexpensive to manufacture, such that it is considered a single-use, disposable item.

In operation and with reference to FIG. 4, pressurized fluids are delivered along the full length of endoscope proximal shaft **112** to endoscope distal tip **120** on demand, under the control of electronics located within operator console **122**, in similar fashion as described in reference to the endoscopic system **100** of FIG. 1. However, the inclusion of multiple fluid sources **410** in the endoscopic system **100** allows multiple fluid types, such as saline, irrigation liquids, medication, or dyes, to be delivered, singly or mixed with one another, to imaging endoscope **110**, under the control of operator console **122** and in combination with handheld manual controller **116** for controlling pump **128** and the pinch valves of tubing sub-assembly **412**. Furthermore, endoscope proximal connector **114** may include multiple fluid channels **212** and fluid reservoir **130**, as described in reference to FIG. 2 or, optionally, may include a greater or lesser number of fluid channels **212** and not include fluid reservoir **130**.

FIG. 5 illustrates a perspective view of a multi-fluid endoscopic system **500** in accordance with a third embodiment of the invention. Multi-fluid endoscopic system **500** includes imaging endoscope **110** that is connected to operator console **122** via endoscope proximal connector **114**, as described in reference to FIGS. 1 and 2. Multi-fluid endoscopic system **400** also includes multiple fluid sources **410**, e.g., fluid source **410a**, **410b**, and **410c**, as described in reference to FIG. 4. However, instead of including tubing sub-assembly **412**, each fluid source **410** has its own dedicated length of tubing **126** and dedicated pump **128** that feed endoscope proximal connector **114** of imaging endoscope **110**. For example, fluid source **410a** is fluidly connected to endoscope proximal connector **114** via a length of tubing **126a** that passes through pump **128a**, fluid source **410b** is fluidly connected to endoscope proximal connector **114** via a length of tubing **126b** that passes through pump **128b**, and fluid source **410c** is fluidly connected to endoscope proximal connector **114** via a length of tubing **126c** that passes through pump **128c**, as shown in FIG. 5. Each fluid source **410**, therefore, has its own dedicated fluid channel **212** and pinch valve **214** within endoscope proximal connector **114**. The dedicated fluid channels **212** pass along the full length of endoscope proximal shaft **112** to endoscope distal tip **120**.

In operation and with reference to FIG. 5, pressurized fluids are delivered along the full length of endoscope proximal shaft **112** to endoscope distal tip **120** on demand, under the control of electronics located within operator console **122**,

in similar fashion as described in reference to multi-fluid endoscopic system **100** of FIG. 1. However, the inclusion of multiple fluid sources **410** in multi-fluid endoscopic system **100** allows multiple fluid types, such as saline, irrigation liquids, medication, or dyes, to be delivered via a dedicated fluid channel **212** to imaging endoscope **110**, under the control of operator console **122**, in combination with handheld manual controller **116**, for controlling pumps **128a**, **128b**, and **128c** and associated pinch valves **214a**, **214b**, and **214c** within endoscope proximal connector **114**. Optionally, endoscope proximal connector **114** may not include fluid reservoir **130**.

FIG. 6 illustrates a perspective view of handheld manual controller **116** that includes a local fluid reservoir in accordance with another embodiment of the invention. FIG. 6 shows that handheld manual controller **116** includes a controller housing **610** formed of a suitably lightweight, rigid material, such as molded plastic. Controller housing **610** is electrically, mechanically, and fluidly connected, at one end, to endoscope proximal shaft **112** and, at an opposite end, to endoscope distal shaft **118**. Mounted within controller housing **610** of handheld manual controller **116** are a plurality of control buttons **612** that allow the physician to manipulate the functions of the endoscope, such as taking a picture, activating light, activating water, activating air, or activating suction at endoscope distal tip **120**. A plurality of rotary knobs **614** control the articulation of endoscope distal tip **120** for advancing into the patient, and a working channel access port **616** allows the insertion of a therapeutic or diagnostic instrument into the working channel of endoscope distal shaft **118**.

In the example shown in FIG. 6, handheld manual controller **116** provides an alternative to having a fluid reservoir located within endoscope proximal connector **114**, such as fluid reservoir **130**, as described in reference to FIGS. 1 and 2. In this example, handheld manual controller **116** further includes an integrated fluid reservoir **618** that has an associated fluid activation button **620**, which provides a conveniently located mechanism for activating the delivery of fluid from integrated fluid reservoir **618**. Integrated fluid reservoir **618** is described in more detail in reference to FIG. 7.

FIG. 7 illustrates a top view of an exemplary integrated fluid reservoir **618** that is installed, optionally, within handheld manual controller **116**. Integrated fluid reservoir **618** includes a fluid bladder **710** surrounded on at least two opposite sides by a water bladder **712**. The contacting surfaces between fluid bladder **710** and water bladder **712** are represented by a pressure interface **714**. The combination of fluid bladder **710** and water bladder **712** that form integrated fluid reservoir **618** is installed into a recessed cavity within controller housing **610** of handheld manual controller **116**.

Fluid bladder **710** is fluidly connected to a fluid channel that is fed into and along the full length of endoscope proximal shaft **112** to endoscope distal tip **120**. Fluid bladder **710** is in the form of a disposable, soft, flexible bladder that is easily detachable from within controller housing **610**. Integrated fluid reservoir **618** includes a pinch valve **716** at the outlet of fluid bladder **710** to control the flow of fluid therefrom. Water bladder **712** is also in the form of a soft, flexible bladder; however, water bladder **712** is permanently installed within controller housing **610**. Integrated fluid reservoir **618** includes a pinch valve **718** at the inlet/outlet of water bladder **712** to control the flow of fluid therethrough.

The capacity of liquid held within fluid bladder **710** is relatively small, compared with the capacity of fluid source **124** or fluid sources **410**. Fluid bladder **710** may be sized, for example, to hold a small quantity of irrigation liquids, contrast media, medication, or dyes for marking tissue. An access door (not shown) may be included within controller housing

**610** of handheld manual controller **116** for installing or removing fluid bladder **710** as needed before, after, or during a medical procedure.

Integrated fluid reservoir **618** takes advantage of the supply of, for example, water passing through handheld manual controller **116** from, for example, fluid source **124** of the endoscopic system **100** or fluid sources **410** of the endoscopic systems **400** and **500**. More specifically, the flow of water is able to pass in or out of water bladder **712** and, therefore, cause water bladder **712** to expand or contract. When water bladder **712** is expanded, pressure is created against fluid bladder **710** at the pressure interface **714**. As a result, a pressure mechanism is created, and pressurized fluid is forced out of fluid bladder **710** and down the fluid channel of endoscope distal shaft **118** and delivered to endoscope distal tip **120**. In operation, the user activates the pressure mechanism created by the combination of fluid bladder **710** and water bladder **712** via fluid activation button **620**, which activates any associated pump (not shown) and controls pinch valves **716** and **718** that enable the flow of, for example, water into water bladder **712** and fluid from fluid bladder **710**.

Those skilled in the art will recognize that the method steps of method **300** may be adapted easily to apply to any of the various medical procedures that use various types of fluid sources, such as shown in FIGS. 1 through 7. For example, fluid source **124**, fluid reservoir **130**, fluid sources **410**, and integrated fluid reservoir **618**, as described in reference to the endoscopic systems **100**, **400**, and **500** of the present invention, provide the user with the flexibility of changing fluids either in advance of a procedure or on-the-fly as needed, instead of relying on fixed fluid sources only. Furthermore, the arrangement of fluid sources, pumps, and valves within the endoscopic systems **100**, **400**, and **500** of the present invention provide a controlled fluid delivery rate and a controlled way of mixing fluids.

FIG. 8 shows yet another alternative embodiment of a fluid delivery system for an endoscope. An endoscopic system **100** includes an imaging endoscope **110** having a handheld manual controller **116** that is used by the physician to operate the endoscope and to steer the endoscope distal tip **120**. The proximal end of the endoscope includes a connector **800** that is releasably secured to a reusable console **820**. As will be described in further detail below, the connector **800** supplies liquids to various lumens in the endoscope in order to perform such functions as bolus wash, jet wash, lens wash, as well as providing vacuum and insufflation. The connector **800** is fluidly coupled to a reservoir **810** including a liquid such as water or saline for delivery to the patient. The connector **800** also includes a U-shaped loop of tubing **830** which engages the rollers of a peristaltic pump **840** for providing fluid pressure to the liquid in the reservoir **810** such that it can be selectively delivered to the lumens of endoscope to perform the desired tasks. The connector **800** is also connected via a tube to a vacuum collection jar **850** that captures retrieved aspirated liquids, debris, tissue samples, etc., from the endoscope.

FIGS. 9A and 9B illustrate further detail of one embodiment of the proximal connector **800**. In the example shown, the connector **800** is made from a molded housing having a front and rear half that are joined to a molded fluid manifold. The connector **800** is sufficiently inexpensive to manufacture such that it can be a disposable item. However, the connector design could also be made to withstand repeated disinfection procedures that are performed with reusable endoscopes.

As shown in FIG. 9A, the proximal connector **800** includes a pair of ports **860**, **862** that receive water from and return water to the fluid reservoir **810** shown in FIG. 8. The reservoir

11

is secured to the ports **860**, **862** with a pair of retaining detents **870**, **872** that engage cooperating elements on the reservoir. The proximal connector **800** also includes one or more ergonomic hand grips **880** that facilitate the insertion and removal of the proximal connector **800** from the console **820**. As shown in FIG. 9B, the proximal connector **800** includes a vacuum port **890** that is connected by a flexible tubing (not shown) to the vacuum collection jar **850**. The U-shaped tubing **830** receives fluid from the fluid input port **860** and delivers it under pressure to a fluid manifold tube (not shown) within the connector.

The rear surface of the connector **800** is shown in FIG. 9C. The rear surface includes one or more bosses **900**, **902**, **904** that are received on corresponding guide pegs (not shown) on the console **820** in order to aid in the placement of the proximal connector on the console. In addition, the proximal connector **800** also includes a number of valve spools **910**, **912**, **914**, **916** that are selectively actuated by an electromagnetic, hydraulic, pneumatic, or other actuator types in order to direct fluids within the manifold to various lumens in the endoscope. An electrical connector **930** is seated within an outwardly extending rim **932** on the rear surface of the proximal connector **800**. The connector **930** serves to connect electrical components within the endoscope to a corresponding electrical connector on the console.

FIG. 10A illustrates the internal components of the proximal connector **800**. The proximal connector includes a manifold **920** including a number of ports **922**, **924**, **926** that are activated by valve spools to selectively deliver pressurized liquid to various lumens of the endoscope. In the embodiment shown, the port **922** delivers liquid for the bolus wash in the endoscope, a port **924** delivers liquid for a lens wash and a port **926** delivers liquid for a jet wash.

The proximal end of the endoscope shaft fits within a receiving portion **940** of the proximal connector **800**. The receiving portion **940** includes a number of ribs **950** that retain the proximal end of the shaft such that it cannot be easily pulled from the connector **800**. In one embodiment, the receiving portion includes an anti-rotation boss **952** that extends through a hole in the endoscope shaft such that the shaft cannot be rotated within the connector.

A cover **960** is placed over the rear surface of electrical connector **930** to secure the connector **930** with the rear surface of the connector and to act as a splash guard. As is best shown in FIG. 10B, the circuit board **930** is held to the rear surface of the connector **800** behind a lip of the outwardly extending rim **932** on the rear surface of the connector **800**. The rim has an opening that exposes the contacts on the connector and a lip that is sized to be smaller than the connector **930**. The cover **960** has an outwardly extending rim **962** that fits within the rim **932** in order to compress the circuit board against the inside surface of the outer rim **932** when the cover **960** is secured to the rear surface of the proximal connector **800**.

A series of molded channels **970** operate to guide the various tubes or lumens in the endoscope to the ports **922**, **924**, and **926** that provide fluids to the endoscope as well as a tube that it is connected to. A port **930** provides insufflation gas to the endoscope.

The proximal connector **800** also includes a four-way port **980**. The port **980** directs fluids and air/vacuum to various lumens within the proximal connector **800**. The port **980** includes a port **982** that is oriented generally in line with the endoscope and is connected to a working channel lumen of the endoscope (not shown). A port **984** extends in a direction perpendicular to the port **982** and in the embodiment shown is

12

connected via a tube (not shown) to the port **922** that supplies water to the port **982** for a bolus wash.

A port **986** is generally in line with the port **982** and is fluidly coupled by a tube (not shown) to a bolus wash over-pressure valve **990** as will be explained in further detail below. In addition, the port **980** includes a fourth port (not shown) positioned in line with the working channel and beneath the port **986** that is coupled by a tube (not shown) to a vacuum port (also not shown).

FIG. 11A illustrates further detail of the manifold **920** within the proximal connector. In the embodiment shown, the manifold is molded as a separate piece and is joined to front and rear halves of the proximal connector **800**. The manifold **920** includes a common tube **1000** which is fluidly connected to each of the ports **922**, **924** and **926**. In addition, the tube **1000** includes a port **1002** that continually delivers a cooling liquid through a lumen to a heat exchanger (not shown) within the distal tip of the endoscope in order to cool the illumination devices. In addition, the manifold **920** includes a port **1004** which receives the cooling liquid back from the heat exchanger and supplies it to the port **862** for return to the liquid reservoir.

FIG. 11B illustrates how the U-shaped flexible tubing **830** is secured within two ports **832**, **834** on the top of the manifold. The port **832** is fluidly coupled to the port **860** that receives liquid from the fluid reservoir. The port **834** is fluidly coupled to the tube **1000** in the manifold **920**. The tubing **830** is preferably made of propylene or other flexible material that can be pressurized by the rollers peristaltic pump **840** on the console **820**.

FIG. 12 illustrates further detail of the valve spools within the ports connected to the manifold. As indicated above, the manifold includes a tube **1000** that contains a pressurized liquid to deliver to each of the various ports. In each of the liquid ports, for example, port **922**, liquid within the tube **1000** flows through a cylinder **1010** having an opening **1012** that fluidly connects the cylinder **1010** with the tube **1000**. The cylinder **1010** has a first diameter in the space between the port **922** and the tube **1000** and a larger diameter in a region **1016** occupying the remainder of the cylinder. A generally cylindrical valve spool, such as valve spool **916**, is slidably received within the cylinder **1010**. The valve spool includes a pair of O-rings **1018**, **1019**. The O-ring **1018** has a smaller diameter that is received within the smaller diameter section **1014** of the cylinder **1010**. Moving the O-ring **1018** into the smaller diameter section **1014** seals the port **922** from receiving fluids from the tube **1000**. Conversely, retracting the valve spool in the cylinder **1010** creates a fluid path between the tube **1000** and the port **922** when the O-ring **1018** is below the port **922** as shown in FIG. 12. At the transition of the larger and smaller diameters of the cylinder, the cylinder is chamfered at an area **1026** to prevent the O-ring **1018** from becoming sheared as the valve spool assembly is moved in and out of the cylinder **1010**. In one embodiment of the invention, the chamfer is set at approximately 30 degrees.

The valve spool also includes a notched section **1020** in which a corresponding tab **1022** from the rear half of the proximal connector is fitted thereby retaining the valve spool in the manifold **920**. Finally, the valve spool includes a stepped portion **1024** of a smaller diameter that allows the spool to be grasped by an actuator to move the valve spool in and out of the cylinder **1010**.

FIGS. 13A and 13B illustrate the vacuum valve assembly within the manifold. The vacuum assembly includes a vacuum port **1050** that is connected by a tube (not shown) to a port on the four-way port **980** that is generally in line with the working channel lumen of the endoscope. The valve

13

assembly includes a valve spool **910** having a construction similar to that described above, which is selectively moved by an actuator to provide fluid communication between the vacuum port **1050** and the port **890** that is coupled to the vacuum collection jar. FIG. **13A** also shows the low pressure bolus wash bypass port **990** that is fluidly connected to the vacuum port **890**. If a bolus wash is applied while the physician has a tool in the working channel or while the working channel is blocked, liquid supplied from the manifold will open a valve in the low pressure bolus wash bypass port **990**. By entering the bypass port **990**, the working channel is prevented from becoming pressurized with a liquid that may splash onto a physician or their assistant.

Further detail of the low pressure bolus wash bypass valve is shown in FIG. **14**. The bypass port **990** includes an insert **1060** that secures a ball valve **1070** and biasing spring **1080** in the port **990**. The insert **1060** has a lip that mates with the surface of the ball valve **1070** in the port **990** by virtue of pressure from the spring **1080**. Once the pressure of the bolus wash liquid in the port **990** overcomes the spring force of the spring **1080**, the ball valve **1070** is opened thereby allowing passage of liquid through the insert **1060** and port **990** to the vacuum port **890**. Also shown in FIGS. **13B** and **14**, the manifold also includes a high pressure bypass valve including a ball valve **1100** and spring **1110** that operate to relieve pressure in the manifold tube **1000**. If pressure within the tube **1000** exceeds the spring force of the spring **1110**, ball valve **1100** is forced open thereby opening a fluid channel between the manifold tube **1000** and the low pressure side of the tubing **830**. In some embodiments of the invention, it may be necessary to employ a metal seating ring within the cylinder of the high pressure bypass valve in order to provide proper mating seal between the cylinder and the ball valve **1100**.

As will be appreciated by those of ordinary skill in the art, the present invention is not limited to the configurations of endoscopic systems as described and shown in reference to FIGS. **1** through **15**. For example, the present invention may be used with an endoscope that is steered by actuators in the console in response to commands received from a user input device such as a joystick or other mechanism. Furthermore, the manifold **620** in the connector **800** may also be used to deliver liquid from alternate fluid source either in the proximal connector or the endoscope such as is shown in FIGS. **1** and **6**. Those skilled in the art will appreciate that any arrangement or combination of the fluid delivery mechanisms disclosed herein or others are possible, without departing from the scope of this invention.

The embodiments of the invention in which an exclusive property or privilege is claimed are defined as follows:

1. An endoscope, comprising:
  - a shaft having a flexible distal shaft with a proximal end and a flexible proximal shaft with a distal end, and one or more lumens therein;
  - a handheld controller connected to the shaft between the proximal and distal ends;
  - a connector at a proximal end of the proximal shaft configured to releasably secure the proximal end of the shaft to a control cabinet, wherein the connector is configured to receive fluids from at least two first fluid sources; and
  - a fluid reservoir located externally from the control cabinet and configured to pressurize a second removable fluid source inserted within the fluid reservoir upon receiving fluids from either one of the at least two first fluid sources to deliver fluid from the second removable fluid source.
2. The endoscope of claim **1**, wherein the at least two first fluid sources are external to the endoscope.

14

3. The endoscope of claim **1**, further including a third first fluid source fluidly coupled to the connector at the proximal end of the proximal shaft, wherein the third first fluid source is configured to pressurize the second removable fluid source.

4. The endoscope of claim **1**, wherein the fluid reservoir is located within the handheld controller.

5. The endoscope of claim **1**, wherein the fluid from the at least two first fluid sources is supplied under pressure from separate fluid pumps.

6. The endoscope of **1**, wherein the fluid from the at least two first fluid sources is supplied under pressure from a common fluid pump.

7. The endoscope of claim **6**, wherein the common fluid pump includes a peristaltic pump.

8. The endoscope of claim **1**, the handheld controller further including an access door for opening the fluid reservoir.

9. The endoscope of claim **1**, wherein the fluid reservoir includes a first bladder configured to be pressurized by fluid from either of the two first fluid sources.

10. The endoscope of claim **9**, wherein the second removable fluid source includes a second bladder configured to be pressurized by the first bladder to force a fluid from the second bladder into the shaft.

11. The endoscope of claim **1**, wherein the connector is further configured to fluidly connect the shaft to the control cabinet.

12. A method of delivering one or more fluids to an internal body cavity of a patient, the method comprising:

inserting a portion of an endoscope into a body cavity of a patient, the endoscope comprising a shaft having a proximal end and distal end, and one or more lumens therein; a connector at the proximal end to releasably secure and fluidly connect the proximal end of the shaft to a control cabinet; a handheld controller, external to the control cabinet and connected to the shaft, wherein the connector is configured to receive a first fluid from either one of at least two first fluid sources;

inserting a second removable fluid source containing a second fluid into a fluid reservoir of the handheld controller, the fluid reservoir configured to pressurize the second removable fluid source to deliver the second fluid;

delivering the first fluid from either one of the two first fluid sources into the connector to pressurize the second removable fluid source, thereby delivering the second fluid; and

delivering the second fluid from the second removable fluid source into the patient via the one or more lumens in the endoscope.

13. The method of claim **12**, wherein at least one of the two first fluid sources is external to the endoscope.

14. The method of claim **13**, wherein the first fluid source includes at least three first fluid sources fluidly coupled to the proximal connector.

15. The method of claim **12**, wherein the second fluid includes a stool softening agent.

16. The method of claim **12**, wherein the second fluid includes a tissue contrast dye.

17. The method of claim **12**, wherein delivering the first fluid from either of the two first fluid sources into the connector to pressurize the second removable fluid source to deliver the second fluid comprises delivering the first fluid from either of the two first fluid sources into a bladder of the fluid reservoir.

18. The method of claim **12**, wherein the shaft includes a flexible distal shaft and a flexible proximal shaft, the connector being positioned at a proximal end of the proximal shaft.

\* \* \* \* \*



UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : 8,083,671 B2  
APPLICATION NO. : 11/239644  
DATED : December 27, 2011  
INVENTOR(S) : D. R. Boulais et al.

Page 1 of 1

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Title page,

item (75), lines 1-2,

“**Dennis R Boulais**, Danielson, CT (US); **Michael S Banik**, Bolton, MA (US);” should read


--**Dennis R. Boulais**, Danielson, CT (US); **Michael S. Banik**, Bolton, MA (US);--;

item (75), lines 5-6,

“**David W Hoffman**, Concord, MA (US); **John P O’Connor**, Andover, MA (US);” should read

--**David W. Hoffman**, Concord, MA (US); **John P. O’Connor**, Andover, MA (US);--.

Signed and Sealed this  
Twenty-seventh Day of March, 2012

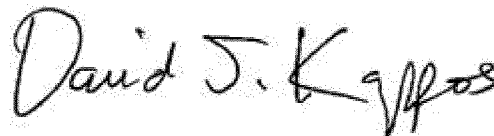

David J. Kappos  
*Director of the United States Patent and Trademark Office*